

LB113283


7471B

INSTRUMENT ID: CV4

Linear

 μ Abs.:

58224

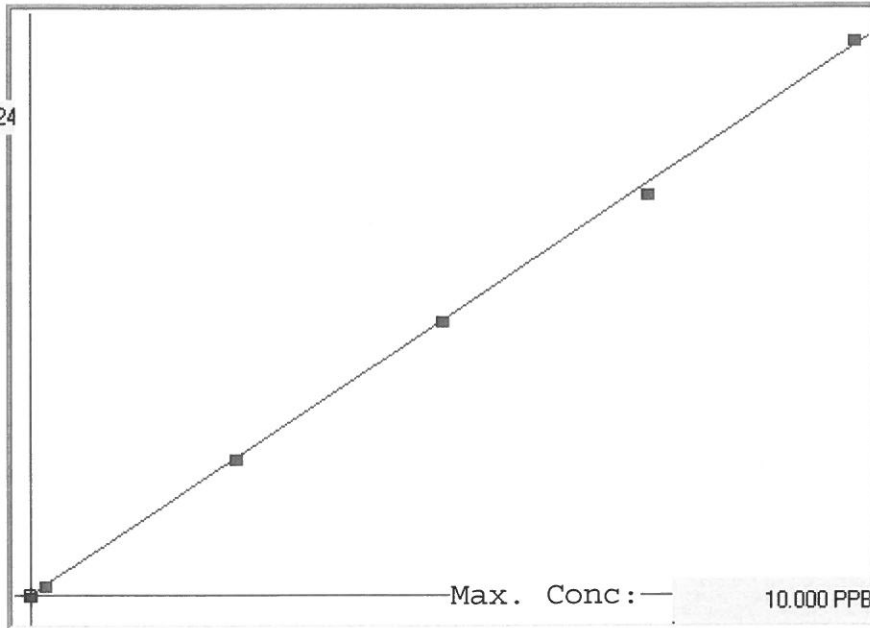

A= 0.0000e+000

B= 1.7342e-004

C= 8.5162e-003

Rho= 0.9997735

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.020	0.020	66	0.000	66					6
0.2	0.200	0.212	0.012	1176	0.0 %	1176					0
2.5	2.500	2.505	0.005	14394	0.0 %	14394					0
5.0	5.000	5.015	0.015	28868	0.0 %	28868					0
7.5	7.500	7.342	-0.158	42286	0.0 %	42286					-2
10.0	10.000	10.106	0.106	58224	0.0 %	58224					1

LB113283 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 26 Feb 2021 14:31:59

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	66	-	0.0000	7471B	PPB	26 Feb 2021 14:33:07	S	Std
0.2 - 1	50.2	1176	-	0.2000	7471B	PPB	26 Feb 2021 14:35:25	S	Std
2.5 - 1	52.5	14394	-	2.5000	7471B	PPB	26 Feb 2021 14:37:42	S	Std
5.0 - 1	55	28868	-	5.0000	7471B	PPB	26 Feb 2021 14:39:59	S	Std
7.5 - 1	57.5	42286	-	7.5000	7471B	PPB	26 Feb 2021 14:42:16	S	Std
10.0 - 1	510	58224	-	10.0000	7471B	PPB	26 Feb 2021 14:44:32	S	Std
ICV17 - 1	ICV17	23455	4.0762	-	7471B	PPB	26 Feb 2021 14:47:19	U	SMPL
ICB17 - 1	ICB17	-44	0.0009	-	7471B	PPB	26 Feb 2021 14:49:34	U	SMPL
CCV42 - 1	CCV42	28655	4.9780	-	7471B	PPB	26 Feb 2021 14:51:49	U	SMPL
CCB42 - 1	CCB42	-57	-0.0014	-	7471B	PPB	26 Feb 2021 14:54:04	U	SMPL
CRA - 1	CRA	1124	0.2034	-	7471B	PPB	26 Feb 2021 14:56:19	U	SMPL
HighStd - 1	HighStd	58596	10.1705	-	7471B	PPB	26 Feb 2021 14:58:34	U	SMPL
ChkStd - 1	ChkStd	40231	6.9855	-	7471B	PPB	26 Feb 2021 15:00:49	U	SMPL
PB134848BL - 1	PBS	-74	-0.0043	-	7471B	PPB	26 Feb 2021 15:03:06	U	SMPL
PB134848BS - 1	LCSS	21663	3.7654	-	7471B	PPB	26 Feb 2021 15:05:22	U	SMPL
M1491-01 - 1	SA-01-022521	1698	0.3030	-	7471B	PPB	26 Feb 2021 15:07:39	U	SMPL
M1499-01 - 1	N-1	3689	0.6483	-	7471B	PPB	26 Feb 2021 15:09:55	U	SMPL
M1501-01 - 1	R-LA-3-7-WC	3048	0.5371	-	7471B	PPB	26 Feb 2021 15:12:13	U	SMPL
M1503-01 - 1	SEDGWICK-AVE	4539	0.7957	-	7471B	PPB	26 Feb 2021 15:14:30	U	SMPL
M1503-01DUP - 1	SEDGWICK-AVEDUP	4839	0.8477	-	7471B	PPB	26 Feb 2021 15:16:46	U	SMPL
CCV43 - 1	CCV43	28897	5.0199	-	7471B	PPB	26 Feb 2021 15:19:01	U	SMPL
CCB43 - 1	CCB43	-39	0.0018	-	7471B	PPB	26 Feb 2021 15:21:17	U	SMPL
M1503-01MS - 1	SEDGWICK-AVEMS	26305	4.5704	-	7471B	PPB	26 Feb 2021 15:23:33	U	SMPL
M1503-01MSD - 1	SEDGWICK-AVEMSD	25456	4.4232	-	7471B	PPB	26 Feb 2021 15:25:48	U	SMPL
M1503-01LX5 - 1		822	0.1511	-	7471B	PPB	26 Feb 2021 15:28:04	U	SMPL
M1503-01A - 1		27515	4.7803	-	7471B	PPB	26 Feb 2021 15:30:20	U	SMPL
CCV44 - 1	CCV44	29050	5.0465	-	7471B	PPB	26 Feb 2021 15:32:36	U	SMPL
CCB44 - 1	CCB44	-52	-0.0005	-	7471B	PPB	26 Feb 2021 15:34:53	U	SMPL