


LB113352

7470A

INSTRUMENT ID: CV2

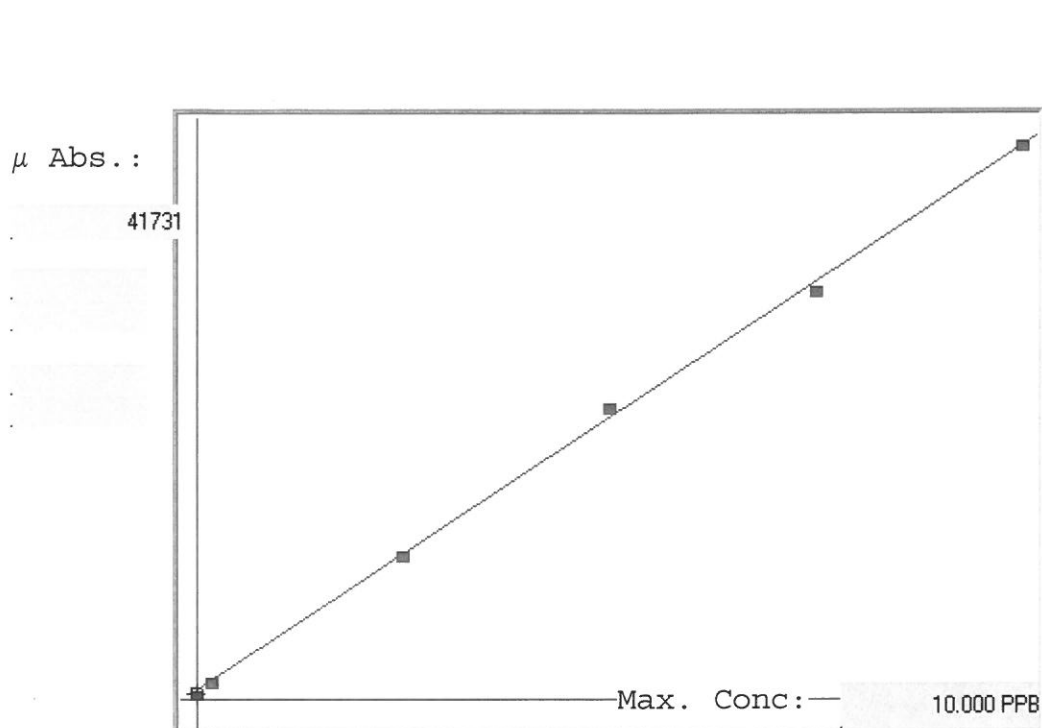

Linear

A= 0.0000e+000

B= 2.4370e-004

C= -1.6282e-001

Rho= 0.9996652

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%b)
0.0	0.000	-0.028	-0.028	555	0.000	555					1
0.2	0.200	0.185	-0.015	1427	0.0 %	1427					8
2.5	2.500	2.484	-0.016	10862	0.0 %	10862					1
5.0	5.000	5.187	0.187	21953	0.0 %	21953					4
7.5	7.500	7.364	-0.136	30887	0.0 %	30887					2
10.0	10.000	10.007	0.007	41731	0.0 %	41731					0

LB113352 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 04 Mar 2021 10:58:31				
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	BD	555	-	0.00007470A	PPB	04 Mar 2021 11:21:10	S	Std
0.2 - 1	50.2	1427	-	0.20007470A	PPB	04 Mar 2021 11:26:04	S	Std
2.5 - 1	52.5	10862	-	2.50007470A	PPB	04 Mar 2021 11:28:20	S	Std
5.0 - 1	55	21953	-	5.00007470A	PPB	04 Mar 2021 11:30:37	S	Std
7.5 - 1	59.5	30887	-	7.50007470A	PPB	04 Mar 2021 11:32:53	S	Std
10.0 - 1	510	41731	-	10.00007470A	PPB	04 Mar 2021 11:35:09	S	Std
ICV24 - 1	ICV24	16238	3.7944	-7470A	PPB	04 Mar 2021 11:37:49	U	SMPL
ICB24 - 1	ICB24	507	-0.0393	-7470A	PPB	04 Mar 2021 11:40:04	U	SMPL
CCV68 - 1	CCV68	21988	5.1956	-7470A	PPB	04 Mar 2021 11:42:18	U	SMPL
CCB68 - 1	CCB68	505	-0.0398	-7470A	PPB	04 Mar 2021 11:44:33	U	SMPL
CRA - 1	CRA	1412	0.1813	-7470A	PPB	04 Mar 2021 11:46:48	U	SMPL
HighStd - 1	HighStd	41974	10.0662	-7470A	PPB	04 Mar 2021 11:49:03	U	SMPL
ChkStd - 1	ChkStd	29501	7.0265	-7470A	PPB	04 Mar 2021 11:51:17	U	SMPL
PB134973BL - 1	PBW	599	-0.0168	-7470A	PPB	04 Mar 2021 11:53:33	U	SMPL
PB134973BS - 1	LCSW	16257	3.7990	-7470A	PPB	04 Mar 2021 11:58:41	U	SMPL
M1458-07 - 1	LOD-MDL-WATER-01-QT1-2021	905	0.0577	-7470A	PPB	04 Mar 2021 12:06:09	U	SMPL
M1458-08 - 1	LOQ-WATER-02-QT1-2021	1399	0.1781	-7470A	PPB	04 Mar 2021 12:08:25	U	SMPL
M1538-01 - 1	1-2-TOTES	415427	HIGH	-7470A	PPB	04 Mar 2021 12:10:42	X	
M1541-02 - 1	FM-786	435	-0.0568	-7470A	PPB	04 Mar 2021 12:15:48	U	SMPL
M1541-02DUP - 1	FM-786DUP	302	-0.0892	-7470A	PPB	04 Mar 2021 12:18:03	U	SMPL
CCV69 - 1	CCV69	21456	5.0660	-7470A	PPB	04 Mar 2021 12:20:18	U	SMPL
CCB69 - 1	CCB69	481	-0.0456	-7470A	PPB	04 Mar 2021 12:22:33	U	SMPL
M1541-02MS - 1	FM-786MS	16765	3.9228	-7470A	PPB	04 Mar 2021 12:24:48	U	SMPL
M1541-02MSD - 1	FM-786MSD	17330	4.0605	-7470A	PPB	04 Mar 2021 12:27:03	U	SMPL
M1538-01DLX10 - 1		77884	18.8174	-7470A	PPB	04 Mar 2021 12:29:19	U	SMPL
M1541-02LX5 - 1		275	-0.0958	-7470A	PPB	04 Mar 2021 12:31:34	U	SMPL
M1541-02A - 1		17065	3.9959	-7470A	PPB	04 Mar 2021 12:33:52	U	SMPL
M1538-01DL2X50 - 1		17183	4.0247	-7470A	PPB	04 Mar 2021 12:36:08	U	SMPL
CCV70 - 1	CCV70	21584	5.0972	-7470A	PPB	04 Mar 2021 12:38:24	U	SMPL
CCB70 - 1	CCB70	602	-0.0161	-7470A	PPB	04 Mar 2021 12:43:34	U	SMPL