


LB113357

SFAM01.1

INSTRUMENT ID: CV1

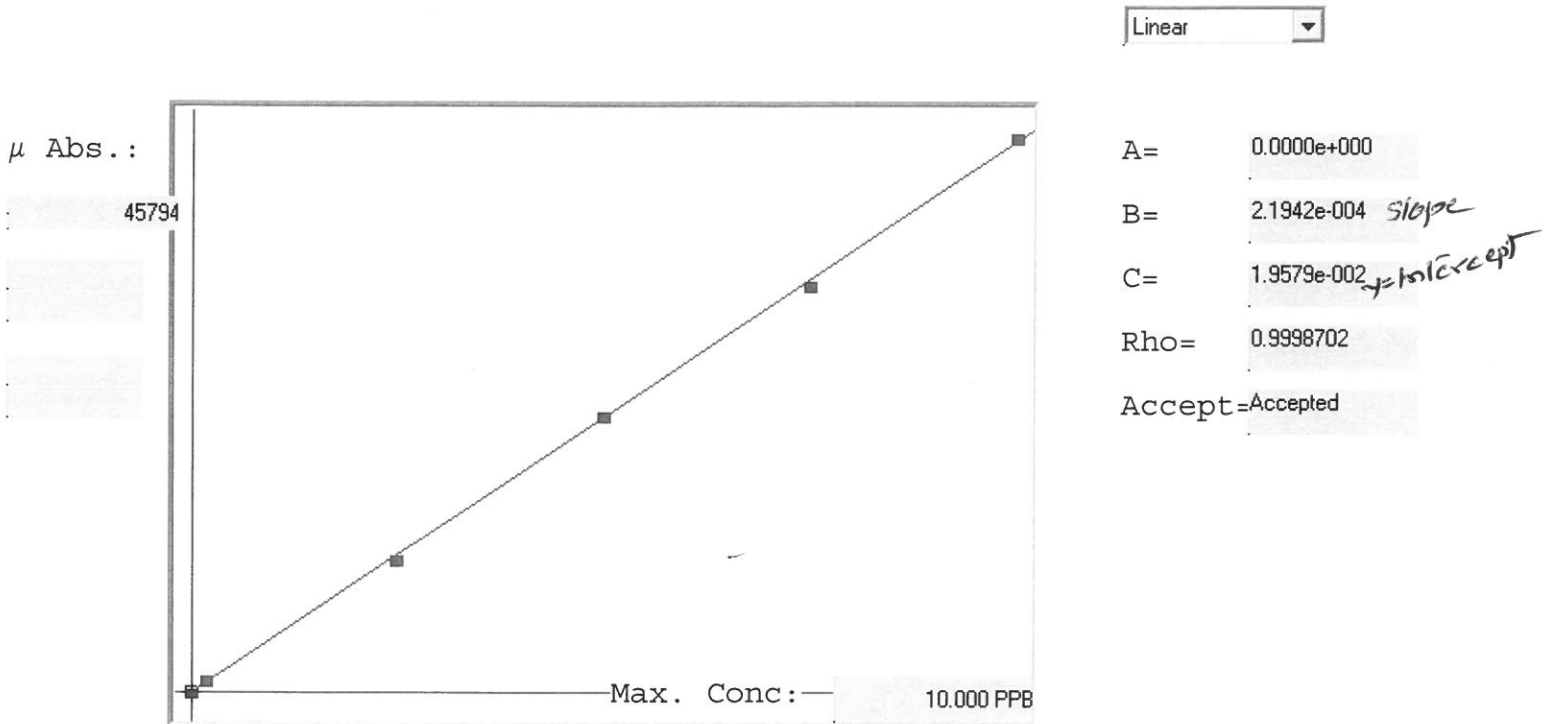

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0/0
0.00	0.000	0.036	0.036	73	0.000	73					-
0.05	0.050					332					-
0.20	0.200	0.229	0.029	956	0.0 %	956					15
2.50	2.500	2.426	-0.074	10969	0.0 %	10969					-3
5.00	5.000	5.031	0.031	22839	0.0 %	22839					1
7.50	7.500	7.410	-0.090	33681	0.0 %	33681					-1
10.0	10.000	10.068	0.068	45794	0.0 %	45794					1

LB113357
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	73	-		0 SFAM01.1	PPB	3/4/2021 13:40	Std
	0.2 S01	956	-		0.2 SFAM01.1	PPB	3/4/2021 13:43	Std
	2.5 S02	10969	-		2.5 SFAM01.1	PPB	3/4/2021 13:45	Std
	5 S03	22839	-		5 SFAM01.1	PPB	3/4/2021 13:47	Std
	7.5 S04	33681	-		7.5 SFAM01.1	PPB	3/4/2021 13:50	Std
	10 S05	45794	-		10 SFAM01.1	PPB	3/4/2021 13:52	Std
ICV017	ICV017	17619	3.8856 -		SFAM01.1	PPB	3/4/2021 13:55	SMPL
ICB017	ICB017	0	0.0196 -		SFAM01.1	PPB	3/4/2021 13:57	SMPL
CCV071	CCV071	22697	4.9998 -		SFAM01.1	PPB	3/4/2021 13:59	SMPL
CCB071	CCB071	7	0.0211 -		SFAM01.1	PPB	3/4/2021 14:01	SMPL
PB134974BL	PBW974	58	0.0323 -		SFAM01.1	PPB	3/4/2021 14:04	SMPL
M1495-07	X3103	4538	1.0153 -		SFAM01.1	PPB	3/4/2021 14:08	SMPL
M1495-08	X3103D	4579	1.0243 -		SFAM01.1	PPB	3/4/2021 14:10	SMPL
M1495-09	X3103S	9119	2.0205 -		SFAM01.1	PPB	3/4/2021 14:15	SMPL
CCV072	CCV072	22691	4.9985 -		SFAM01.1	PPB	3/4/2021 14:20	SMPL
CCB072	CCB072	4	0.0205 -		SFAM01.1	PPB	3/4/2021 14:22	SMPL