


LB113893

7470A

INSTRUMENT ID: CV1

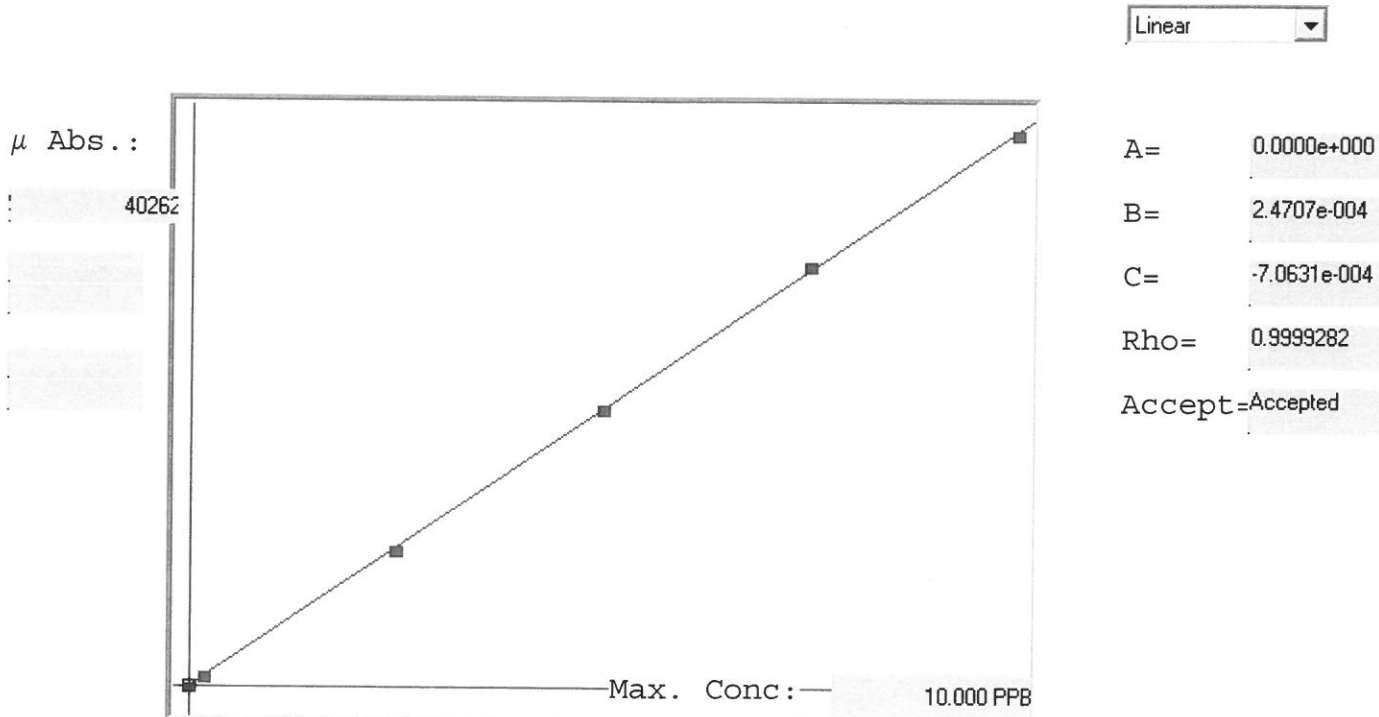

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.006	0.006	27	0.000	27					-
0.2	0.200	0.205	0.005	833	0.0 %	833					3
2.5	2.500	2.463	-0.037	9970	0.0 %	9970					-1
5.0	5.000	4.994	-0.006	20214	0.0 %	20214					0
7.5	7.500	7.586	0.086	30707	0.0 %	30707					1
10.0	10.000	9.947	-0.053	40262	0.0 %	40262					-1

LB113393 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 08 Mar 2021 10:52:11				
Sample ID	Extended ID	µ Abs	Conc	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	27	-	0.00007470A	PPB	08 Mar 2021 11:02:37	S	Std
0.2 - 1	50.2	833	-	0.20007470A	PPB	08 Mar 2021 11:04:54	S	Std
2.5 - 1	52.5	9970	-	2.50007470A	PPB	08 Mar 2021 11:07:10	S	Std
5.0 - 1		20214	-	5.00007470A	PPB	08 Mar 2021 11:09:27	S	Std
7.5 - 1	55	30707	-	7.50007470A	PPB	08 Mar 2021 11:11:43	S	Std
10.0 - 1	57.5	40262	-	10.00007470A	PPB	08 Mar 2021 11:16:32	S	Std
ICV27 - 1	ICV27	15610	3.8560	-7470A	PPB	08 Mar 2021 11:19:12	U	SMPL
ICB27 - 1	ICB27	-59	-0.0153	-7470A	PPB	08 Mar 2021 11:21:26	U	SMPL
CCV84 - 1	CCV84	20500	5.0642	-7470A	PPB	08 Mar 2021 11:23:41	U	SMPL
CCB84 - 1	CCB84	-62	-0.0160	-7470A	PPB	08 Mar 2021 11:25:56	U	SMPL
CRA - 1	CRA	806	0.1984	-7470A	PPB	08 Mar 2021 11:28:11	U	SMPL
HighStd - 1	HighStd	40226	9.9379	-7470A	PPB	08 Mar 2021 11:30:26	U	SMPL
ChkStd - 1	ChkStd	28883	7.1354	-7470A	PPB	08 Mar 2021 11:32:41	U	SMPL
PB135029BL - 1	PBW	-47	-0.0123	-7470A	PPB	08 Mar 2021 11:34:57	U	SMPL
PB135029BS - 1	LCSW	14909	3.6828	-7470A	PPB	08 Mar 2021 11:39:47	U	SMPL
M1552-01 - 1	24368	-12	-0.0037	-7470A	PPB	08 Mar 2021 11:42:03	U	SMPL
M1553-03 - 1	347	23	0.0050	-7470A	PPB	08 Mar 2021 11:44:19	U	SMPL
M1553-03DUP - 1	347DUP	49	0.0114	-7470A	PPB	08 Mar 2021 11:46:36	U	SMPL
M1553-03MS - 1	347MS	14866	3.6722	-7470A	PPB	08 Mar 2021 11:51:45	U	SMPL
M1553-03MSD - 1	347MSD	14749	3.6433	-7470A	PPB	08 Mar 2021 11:53:59	U	SMPL
CCV85 - 1	CCV85	20500	5.0642	-7470A	PPB	08 Mar 2021 11:56:15	U	SMPL
CCB85 - 1	CCB85	-59	-0.0153	-7470A	PPB	08 Mar 2021 11:58:30	U	SMPL
PB135031BL - 1	PBW	-5	-0.0019	-7470A	PPB	08 Mar 2021 12:00:46	U	SMPL
PB135031BS - 1	LCSW	14919	3.6853	-7470A	PPB	08 Mar 2021 12:05:34	U	SMPL
M1458-07 - 1	LOD-MDL-WATER-01-QT1-2021	710	0.1747	-7470A	PPB	08 Mar 2021 12:07:50	U	SMPL
M1458-09 - 1	MDL-WATER-03-QT1-2021	198	0.0482	-7470A	PPB	08 Mar 2021 12:10:05	U	SMPL
M1575-01 - 1	IDW-GW803-AQ-030321	55	0.0129	-7470A	PPB	08 Mar 2021 12:12:21	U	SMPL
M1575-02 - 1	IDW-GW804-AQ-030321	73	0.0173	-7470A	PPB	08 Mar 2021 12:14:37	U	SMPL
M1575-03 - 1	IDW-GW805-AQ-030321	51	0.0119	-7470A	PPB	08 Mar 2021 12:16:53	U	SMPL
M1575-04 - 1	IDW-GW806-AQ-030321	29	0.0065	-7470A	PPB	08 Mar 2021 12:19:10	U	SMPL
M1575-05 - 1	IDW-GW807B-AQ-030421	32	0.0072	-7470A	PPB	08 Mar 2021 12:21:27	U	SMPL
M1585-02 - 1	TT-028-IDWGW-20210304	41	0.0094	-7470A	PPB	08 Mar 2021 12:23:43	U	SMPL
CCV86 - 1	CCV86	18317	4.5249	-7470A	PPB	08 Mar 2021 12:25:58	U	SMPL
CCB86 - 1	CCB86	-132	-0.0333	-7470A	PPB	08 Mar 2021 12:28:14	U	SMPL
M1585-02DUP - 1	TT-028-IDWGW-20210304DUP	10	0.0018	-7470A	PPB	08 Mar 2021 12:30:30	U	SMPL
M1585-02MS - 1	TT-028-IDWGW-20210304MS	14651	3.6191	-7470A	PPB	08 Mar 2021 12:35:18	U	SMPL
M1585-02MSD - 1	TT-028-IDWGW-20210304MSD	14819	3.6606	-7470A	PPB	08 Mar 2021 12:37:33	U	SMPL
PB135029TB - 1	PB134976TB	-6	-0.0022	-7470A	PPB	08 Mar 2021 12:42:25	U	SMPL
M1553-03LX5 - 1		17	0.0035	-7470A	PPB	08 Mar 2021 12:44:41	U	SMPL
M1553-03A - 1		17086	4.2207	-7470A	PPB	08 Mar 2021 12:46:57	U	SMPL
M1585-02LX5 - 1		-18	-0.0052	-7470A	PPB	08 Mar 2021 12:49:14	U	SMPL
M1585-02A - 1		17044	4.2103	-7470A	PPB	08 Mar 2021 12:51:31	U	SMPL
CCV87 - 1	CCV87	20535	5.0729	-7470A	PPB	08 Mar 2021 12:53:48	U	SMPL
CCB87 - 1	CCB87	-26	-0.0071	-7470A	PPB	08 Mar 2021 12:56:04	U	SMPL