


LB113406

7470A

INSTRUMENT ID: CV2

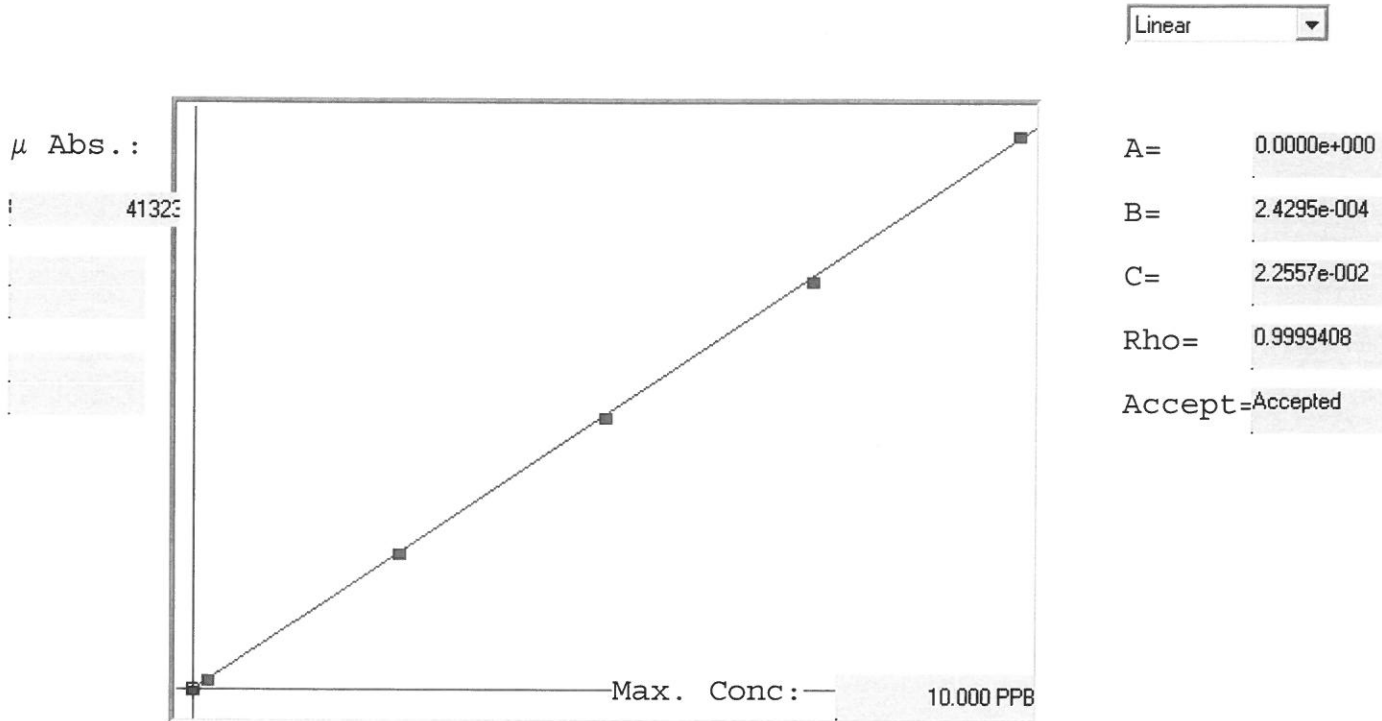

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	90D
0.0	0.000	0.029	0.029	28	0.000	28					
0.2	0.200	0.207	0.007	758	0.0 %	758					
2.5	2.500	2.500	-0.000	10196	0.0 %	10196					
5.0	5.000	4.959	-0.041	20318	0.0 %	20318					
7.5	7.500	7.443	-0.057	30544	0.0 %	30544					
10.0	10.000	10.062	0.062	41323	0.0 %	41323					

90D
4
0
-1
-1
1

LB113406 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 09 Mar 2021 09:53:55					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	28	-	0.0000	7470A	PPB	09 Mar 2021 10:01:11	S	Std
0.2 - 1	SO-2	758	-	0.2000	7470A	PPB	09 Mar 2021 10:03:28	S	Std
2.5 - 1	52.5	10196	-	2.5000	7470A	PPB	09 Mar 2021 10:05:45	S	Std
5.0 - 1	55	20318	-	5.0000	7470A	PPB	09 Mar 2021 10:08:02	S	Std
7.5 - 1	57.5	30544	-	7.5000	7470A	PPB	09 Mar 2021 10:10:18	S	Std
10.0 - 1	510	41323	-	10.0000	7470A	PPB	09 Mar 2021 10:12:34	S	Std
ICV28 - 1	ICV28	15072	3.6843	-	7470A	PPB	09 Mar 2021 10:15:22	U	SMPL
ICB28 - 1	ICB28	-35	0.0141	-	7470A	PPB	09 Mar 2021 10:17:37	U	SMPL
CCV88 - 1	CCV88	20836	5.0847	-	7470A	PPB	09 Mar 2021 10:19:51	U	SMPL
CCB88 - 1	CCB88	-43	0.0121	-	7470A	PPB	09 Mar 2021 10:22:06	U	SMPL
CRA - 1	CRA	755	0.2060	-	7470A	PPB	09 Mar 2021 10:24:21	U	SMPL
HighStd - 1	HighStd	41370	10.0735	-	7470A	PPB	09 Mar 2021 10:26:36	U	SMPL
ChkStd - 1	ChkStd	29429	7.1724	-	7470A	PPB	09 Mar 2021 10:28:51	U	SMPL
PB135045BL - 1	PBW	-61	0.0077	-	7470A	PPB	09 Mar 2021 10:31:07	U	SMPL
PB135045BS - 1	LCSW	17489	4.2715	-	7470A	PPB	09 Mar 2021 10:35:57	U	SMPL
M1576-08 - 1	IDW-GW803-SO-030421	-19	0.0179	-	7470A	PPB	09 Mar 2021 10:38:13	U	SMPL
M1576-08DUP - 1	IDW-GW803-SO-030421DUP	29	0.0296	-	7470A	PPB	09 Mar 2021 10:40:30	U	SMPL
M1576-08MS - 1	IDW-GW803-SO-030421MS	14970	3.6596	-	7470A	PPB	09 Mar 2021 10:42:47	U	SMPL
M1576-08MSD - 1	IDW-GW803-SO-030421MSD	15182	3.7111	-	7470A	PPB	09 Mar 2021 10:45:03	U	SMPL
M1576-09 - 1	IDW-GW804-SO-030421	-17	0.0184	-	7470A	PPB	09 Mar 2021 10:47:18	U	SMPL
CCV89 - 1	CCV89	20533	5.0111	-	7470A	PPB	09 Mar 2021 10:49:33	U	SMPL
CCB89 - 1	CCB89	-31	0.0150	-	7470A	PPB	09 Mar 2021 10:51:49	U	SMPL
M1576-10 - 1	IDW-GW805-SO-030421	38	0.0318	-	7470A	PPB	09 Mar 2021 10:54:04	U	SMPL
M1576-11 - 1	IDW-GW806-SO-030421	31	0.0301	-	7470A	PPB	09 Mar 2021 10:56:19	U	SMPL
M1576-12 - 1	IDW-GW807B-SO-030421	49	0.0345	-	7470A	PPB	09 Mar 2021 10:58:34	U	SMPL
M1580-01 - 1	03-05A	43	0.0330	-	7470A	PPB	09 Mar 2021 11:00:49	U	SMPL
M1580-02 - 1	03-05B	40	0.0323	-	7470A	PPB	09 Mar 2021 11:03:05	U	SMPL
M1580-03 - 1	03-05C	45	0.0335	-	7470A	PPB	09 Mar 2021 11:05:21	U	SMPL
M1580-04 - 1	03-05D	39	0.0320	-	7470A	PPB	09 Mar 2021 11:07:37	U	SMPL
M1581-01 - 1	03-05E	35	0.0311	-	7470A	PPB	09 Mar 2021 11:09:54	U	SMPL
M1581-02 - 1	03-05F	44	0.0332	-	7470A	PPB	09 Mar 2021 11:12:11	U	SMPL
M1581-03 - 1	03-05G	55	0.0359	-	7470A	PPB	09 Mar 2021 11:14:26	U	SMPL
CCV90 - 1	CCV90	20605	5.0286	-	7470A	PPB	09 Mar 2021 11:16:42	U	SMPL
CCB90 - 1	CCB90	-29	0.0155	-	7470A	PPB	09 Mar 2021 11:18:57	U	SMPL
M1581-04 - 1	03-05H	40	0.0323	-	7470A	PPB	09 Mar 2021 11:21:13	U	SMPL
M1581-05 - 1	03-05I	25	0.0286	-	7470A	PPB	09 Mar 2021 11:23:28	U	SMPL
M1581-06 - 1	03-05J	36	0.0313	-	7470A	PPB	09 Mar 2021 11:25:43	U	SMPL
PB135045TB - 1	PB135027TB	39	0.0320	-	7470A	PPB	09 Mar 2021 11:27:58	U	SMPL
M1576-08LX5 - 1		37	0.0315	-	7470A	PPB	09 Mar 2021 11:30:14	U	SMPL
M1576-08A - 1		15499	3.7881	-	7470A	PPB	09 Mar 2021 11:32:30	U	SMPL
CCV91 - 1	CCV91	20565	5.0189	-	7470A	PPB	09 Mar 2021 11:34:47	U	SMPL
CCB91 - 1	CCB91	-23	0.0170	-	7470A	PPB	09 Mar 2021 11:37:03	U	SMPL