

LB113428


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

4108E

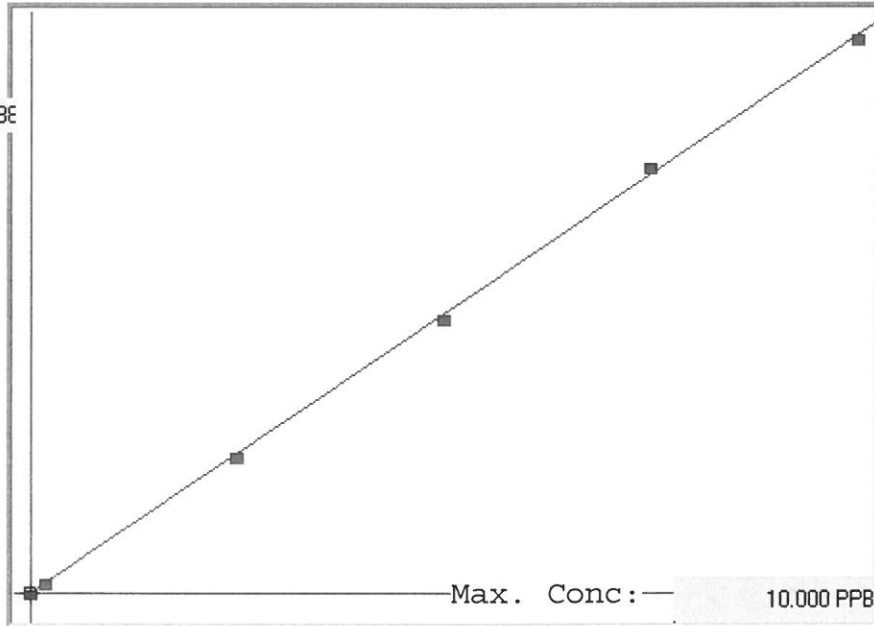

A= 0.0000e+000

B= 2.4148e-004

C= 7.3468e-003

Rho= 0.9998162

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.018	0.018	46	0.000	46					6
0.2	0.200	0.212	0.012	847	0.0 %	847					-2
2.5	2.500	2.451	-0.049	10118	0.0 %	10118					-1
5.0	5.000	4.950	-0.050	20468	0.0 %	20468					2
7.5	7.500	7.640	0.140	31608	0.0 %	31608					-1
10.0	10.000	9.929	-0.071	41088	0.0 %	41088					

LB113428 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 Mar 2021 10:50:30

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	46	-	0.0000	7470A	PPB	10 Mar 2021 10:53:23	S	Std
0.2 - 1	50.2	847	-	0.2000	7470A	PPB	10 Mar 2021 10:55:39	S	Std
2.5 - 1	52.5	10118	-	2.5000	7470A	PPB	10 Mar 2021 10:57:56	S	Std
5.0 - 1	55	20468	-	5.0000	7470A	PPB	10 Mar 2021 11:00:13	S	Std
7.5 - 1	57.5	31608	-	7.5000	7470A	PPB	10 Mar 2021 11:02:29	S	Std
10.0 - 1	510	41088	-	10.0000	7470A	PPB	10 Mar 2021 11:07:20	S	Std
ICV30 - 1	ICV30	15776	3.8169	-	7470A	PPB	10 Mar 2021 11:10:06	U	SMPL
ICB30 - 1	ICB30	-30	0.0001	-	7470A	PPB	10 Mar 2021 11:12:21	U	SMPL
CCV96 - 1	CCV96	20771	5.0231	-	7470A	PPB	10 Mar 2021 11:14:35	U	SMPL
CCB96 - 1	CCB96	-37	-0.0016	-	7470A	PPB	10 Mar 2021 11:16:50	U	SMPL
CRA - 1	CRA	826	0.2068	-	7470A	PPB	10 Mar 2021 11:19:05	U	SMPL
HighStd - 1	HighStd	40797	9.8589	-	7470A	PPB	10 Mar 2021 11:21:19	U	SMPL
ChkStd - 1	ChkStd	29015	7.0138	-	7470A	PPB	10 Mar 2021 11:23:35	U	SMPL
PB135075BL - 1	PBW	-78	-0.0115	-	7470A	PPB	10 Mar 2021 11:25:51	U	SMPL
PB135075BS - 1	LCSW	15760	3.8130	-	7470A	PPB	10 Mar 2021 11:28:07	U	SMPL
M1577-02 - 1	72-11939-VNJ-229	-27	0.0008	-	7470A	PPB	10 Mar 2021 11:30:23	U	SMPL
M1603-04 - 1	31-NORTH	20	0.0122	-	7470A	PPB	10 Mar 2021 11:32:40	U	SMPL
M1603-04DUP - 1	31-NORTHDUP	30	0.0146	-	7470A	PPB	10 Mar 2021 11:34:56	U	SMPL
M1603-04MS - 1	31-NORTHMS	16210	3.9217	-	7470A	PPB	10 Mar 2021 11:37:13	U	SMPL
M1603-04MSD - 1	31-NORTHMSD	16529	3.9987	-	7470A	PPB	10 Mar 2021 11:39:28	U	SMPL
CCV97 - 1	CCV97	20798	5.0296	-	7470A	PPB	10 Mar 2021 11:41:43	U	SMPL
CCB97 - 1	CCB97	-45	-0.0035	-	7470A	PPB	10 Mar 2021 11:43:59	U	SMPL
M1603-05 - 1	32-NORTH	31	0.0148	-	7470A	PPB	10 Mar 2021 11:46:14	U	SMPL
M1603-06 - 1	33-NORTH	22	0.0127	-	7470A	PPB	10 Mar 2021 11:48:29	U	SMPL
PB135075TB - 1	PB135054TB	24	0.0131	-	7470A	PPB	10 Mar 2021 11:50:45	U	SMPL
M1603-04LX5 - 1		29	0.0143	-	7470A	PPB	10 Mar 2021 11:53:00	U	SMPL
M1603-04A - 1		16254	3.9323	-	7470A	PPB	10 Mar 2021 11:55:16	U	SMPL
CCV98 - 1	CCV98	20963	5.0694	-	7470A	PPB	10 Mar 2021 11:57:32	U	SMPL
CCB98 - 1	CCB98	-34	-0.0009	-	7470A	PPB	10 Mar 2021 11:59:48	U	SMPL