


LB113445

7471B

INSTRUMENT ID: CV1

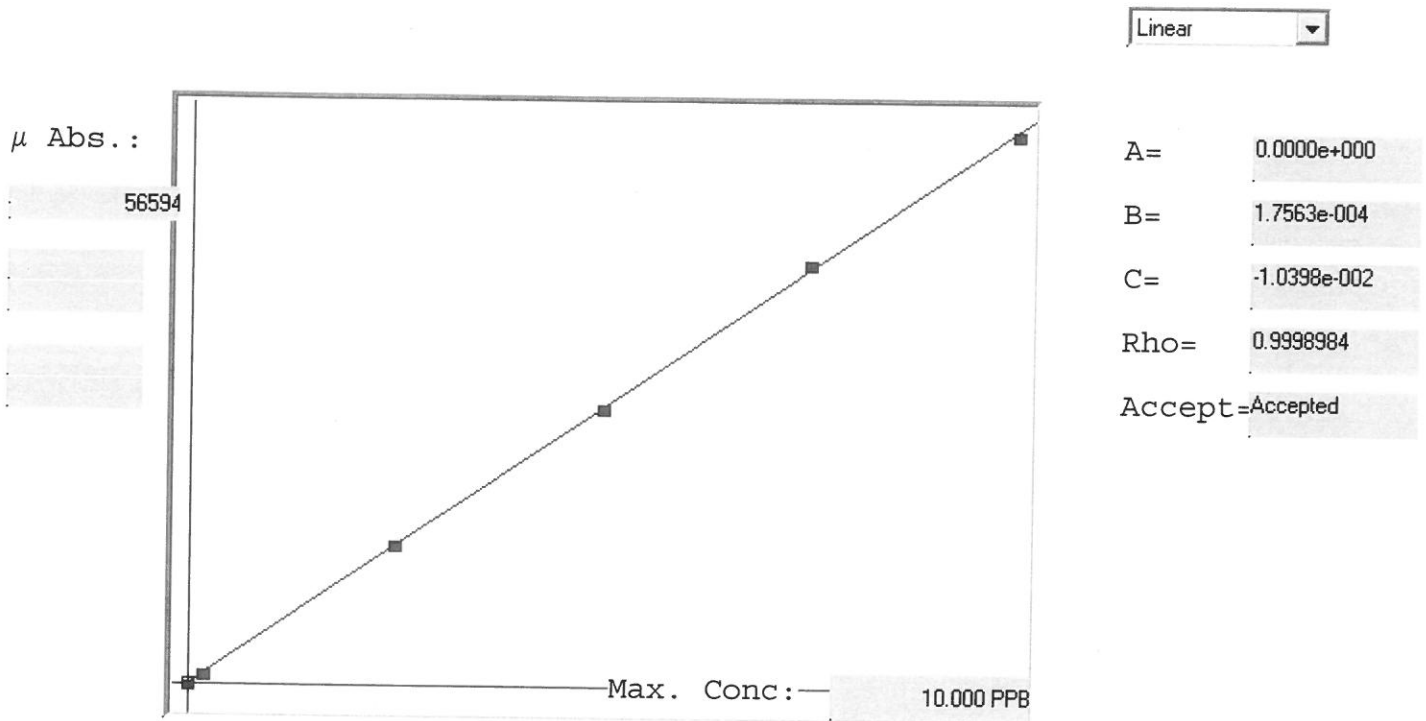

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.004	-0.004	39	0.000	39					
0.2	0.200	0.187	-0.013	1126	0.0 %	1126					-7
2.5	2.500	2.501	0.001	14301	0.0 %	14301					0
5.0	5.000	4.981	-0.019	28419	0.0 %	28419					0
7.5	7.500	7.605	0.105	43361	0.0 %	43361					1
10.0	10.000	9.929	-0.071	56594	0.0 %	56594					-1

LB113445 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 10 Mar 2021 14:57:27

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	39	-	0.0000	7471B	PPB	10 Mar 2021 15:06:10	S	Std
0.2 - 1	50.2	1126	-	0.2000	7471B	PPB	10 Mar 2021 15:08:26	S	Std
2.5 - 1	52.5	14301	-	2.5000	7471B	PPB	10 Mar 2021 15:10:43	S	Std
5.0 - 1	55	28419	-	5.0000	7471B	PPB	10 Mar 2021 15:13:00	S	Std
7.5 - 1	57.5	43361	-	7.5000	7471B	PPB	10 Mar 2021 15:15:16	S	Std
10.0 - 1	510	56594	-	10.0000	7471B	PPB	10 Mar 2021 15:17:32	S	Std
ICV31 - 1	ICV31	22009	3.8550	-	7471B	PPB	10 Mar 2021 15:20:18	U	SMPL
ICB31 - 1	ICB31	-15	-0.0130	-	7471B	PPB	10 Mar 2021 15:22:33	U	SMPL
CCV01 - 1	CCV01	28782	5.0445	-	7471B	PPB	10 Mar 2021 15:24:48	U	SMPL
CCB01 - 1	CCB01	-25	-0.0148	-	7471B	PPB	10 Mar 2021 15:27:03	U	SMPL
CRA - 1	CRA	1123	0.1868	-	7471B	PPB	10 Mar 2021 15:29:18	U	SMPL
HighStd - 1	HighStd	56769	9.9599	-	7471B	PPB	10 Mar 2021 15:31:33	U	SMPL
ChkStd - 1	ChkStd	40464	7.0962	-	7471B	PPB	10 Mar 2021 15:33:48	U	SMPL
PB135076BL - 1	PBS	-59	-0.0208	-	7471B	PPB	10 Mar 2021 15:36:06	U	SMPL
PB135076BS - 1	LCSS	21765	3.8122	-	7471B	PPB	10 Mar 2021 15:38:22	U	SMPL
M1597-01 - 1	AU-06-030821	3726	0.6440	-	7471B	PPB	10 Mar 2021 15:40:38	U	SMPL
M1598-01 - 1	OR-02-030821	1686	0.2857	-	7471B	PPB	10 Mar 2021 15:42:55	U	SMPL
M1599-01 - 1	OK-02-030821	919	0.1510	-	7471B	PPB	10 Mar 2021 15:45:11	U	SMPL
M1600-02 - 1	BIN-4	5385	0.9354	-	7471B	PPB	10 Mar 2021 15:52:47	U	SMPL
M1600-02DUP - 1	BIN-4DUP	5479	0.9519	-	7471B	PPB	10 Mar 2021 15:55:02	U	SMPL
CCV02 - 1	CCV02	28893	5.0640	-	7471B	PPB	10 Mar 2021 15:57:17	U	SMPL
CCB02 - 1	CCB02	-24	-0.0146	-	7471B	PPB	10 Mar 2021 15:59:32	U	SMPL
M1600-02MS - 1	BIN-4MS	25478	4.4643	-	7471B	PPB	10 Mar 2021 16:01:48	U	SMPL
M1600-02MSD - 1	BIN-4MSD	27854	4.8816	-	7471B	PPB	10 Mar 2021 16:04:03	U	SMPL
M1601-02 - 1	BIN-3	4940	0.8572	-	7471B	PPB	10 Mar 2021 16:06:18	U	SMPL
M1602-01 - 1	SU-02-030821	1743	0.2957	-	7471B	PPB	10 Mar 2021 16:08:33	U	SMPL
M1607-01 - 1	NB-07-030921	229	0.0298	-	7471B	PPB	10 Mar 2021 16:10:49	U	SMPL
M1608-01 - 1	HD-02-030921	561	0.0881	-	7471B	PPB	10 Mar 2021 16:13:05	U	SMPL
M1609-01 - 1	TR-05-030921	2505	0.4296	-	7471B	PPB	10 Mar 2021 16:15:21	U	SMPL
M1613-01 - 1	S-1	893	0.1464	-	7471B	PPB	10 Mar 2021 16:17:38	U	SMPL
M1614-01 - 1	FK-BPM-03-021-ABCD	1822	0.3096	-	7471B	PPB	10 Mar 2021 16:19:54	U	SMPL
M1615-01 - 1	FK-BPM-04-015-ABCD	840	0.1371	-	7471B	PPB	10 Mar 2021 16:22:10	U	SMPL
CCV03 - 1	CCV03	29135	5.1065	-	7471B	PPB	10 Mar 2021 16:24:25	U	SMPL
CCB03 - 1	CCB03	-14	-0.0129	-	7471B	PPB	10 Mar 2021 16:26:41	U	SMPL
M1616-01 - 1	TP-19-A	1117	0.1858	-	7471B	PPB	10 Mar 2021 16:28:56	U	SMPL
M1600-02LX5 - 1		1072	0.1779	-	7471B	PPB	10 Mar 2021 16:31:11	U	SMPL
M1600-02A - 1		28079	4.9211	-	7471B	PPB	10 Mar 2021 16:33:27	U	SMPL
CCV04 - 1	CCV04	28905	5.0661	-	7471B	PPB	10 Mar 2021 16:35:42	U	SMPL
CCB04 - 1	CCB04	-13	-0.0127	-	7471B	PPB	10 Mar 2021 16:37:58	U	SMPL