


LB113482

INSTRUMENT ID: CV1

7470A

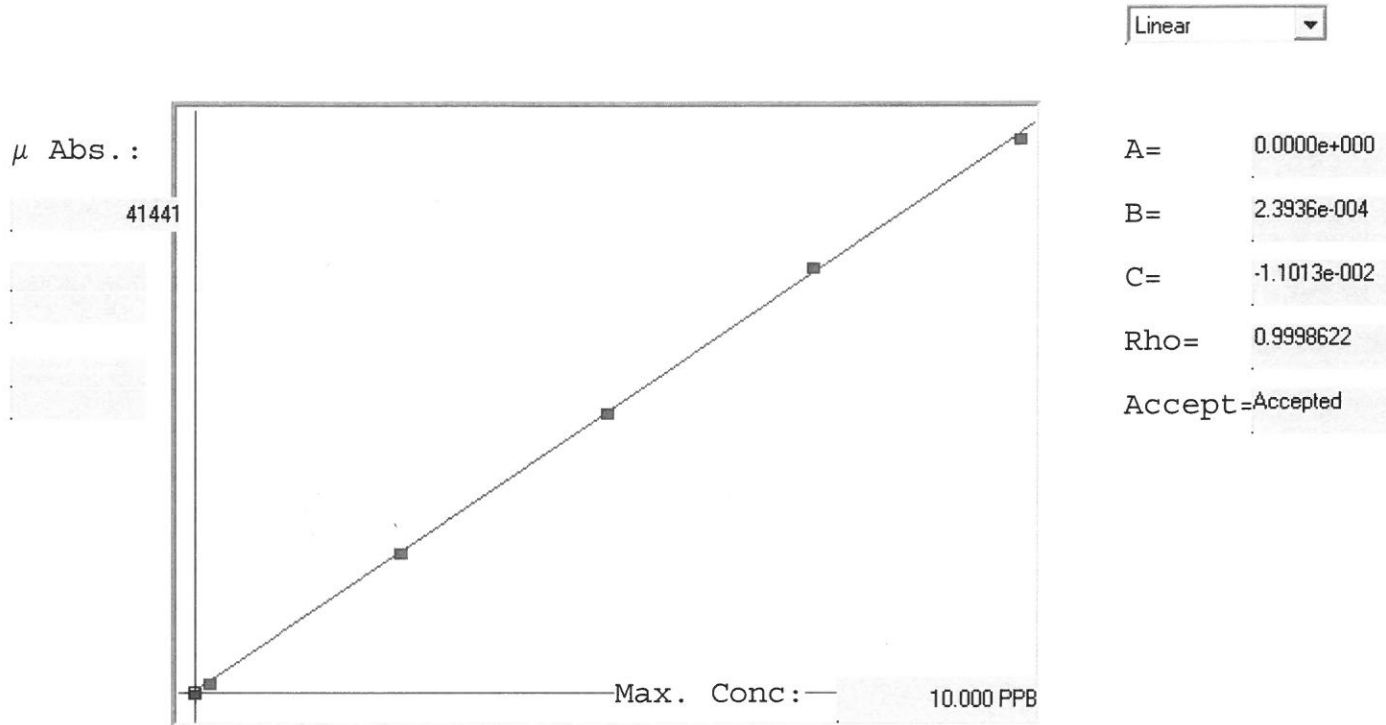

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.002	0.002	54	0.000	54					
0.2	0.200	0.169	-0.031	752	0.0 %	752					
2.5	2.500	2.496	-0.004	10472	0.0 %	10472					
5.0	5.000	5.011	0.011	20981	0.0 %	20981					
7.5	7.500	7.614	0.114	31856	0.0 %	31856					
10.0	10.000	9.908	-0.092	41441	0.0 %	41441					

0/00

-16

0

0

2

-1

LB113482 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Mar 2021 10:51:18

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	54	-	0.0000	7470A	PPB	12 Mar 2021 10:53:11	S	Std
0.2 - 1	50.2	752	-	0.2000	7470A	PPB	12 Mar 2021 10:58:30	S	Std
2.5 - 1	52.5	10472	-	2.5000	7470A	PPB	12 Mar 2021 11:00:46	S	Std
5.0 - 1	55	20981	-	5.0000	7470A	PPB	12 Mar 2021 11:03:03	S	Std
7.5 - 1	55	31856	-	7.5000	7470A	PPB	12 Mar 2021 11:05:20	S	Std
10.0 - 1	510	41441	-	10.0000	7470A	PPB	12 Mar 2021 11:07:35	S	Std
ICV35 - 1	ICV35	15199	3.6270	-	7470A	PPB	12 Mar 2021 11:13:17	U	SMPL
ICB35 - 1	ICB35	76	0.0072	-	7470A	PPB	12 Mar 2021 11:15:32	U	SMPL
CCV12 - 1	CCV12	21343	5.0977	-	7470A	PPB	12 Mar 2021 11:17:47	U	SMPL
CCB12 - 1	CCB12	74	0.0067	-	7470A	PPB	12 Mar 2021 11:20:02	U	SMPL
CRA - 1	CRA	845	0.1912	-	7470A	PPB	12 Mar 2021 11:22:17	U	SMPL
HighStd - 1	HighStd	42544	10.1724	-	7470A	PPB	12 Mar 2021 11:24:32	U	SMPL
ChkStd - 1	ChkStd	30535	7.2979	-	7470A	PPB	12 Mar 2021 11:26:46	U	SMPL
PB135119BL - 1	PBW	173	0.0304	-	7470A	PPB	12 Mar 2021 11:29:02	U	SMPL
PB135119BS - 1	LCSW	16270	3.8834	-	7470A	PPB	12 Mar 2021 11:31:17	U	SMPL
M1565-11 - 1	TP-1	309	0.0630	-	7470A	PPB	12 Mar 2021 11:33:33	U	SMPL
M1565-11DUP - 1	TP-1DUP	359	0.0749	-	7470A	PPB	12 Mar 2021 11:35:49	U	SMPL
M1565-11MS - 1	TP-1MS	15335	3.6596	-	7470A	PPB	12 Mar 2021 11:38:05	U	SMPL
M1565-11MSD - 1	TP-1MSD	15478	3.6938	-	7470A	PPB	12 Mar 2021 11:40:23	U	SMPL
PB135120BL - 1	PBW	49	0.0007	-	7470A	PPB	12 Mar 2021 11:45:13	U	SMPL
CCV13 - 1	CCV13	20842	4.9778	-	7470A	PPB	12 Mar 2021 11:47:28	U	SMPL
CCB13 - 1	CCB13	86	0.0096	-	7470A	PPB	12 Mar 2021 11:49:43	U	SMPL
PB135120BS - 1	LCSW	15261	3.6419	-	7470A	PPB	12 Mar 2021 11:51:59	U	SMPL
M1619-02 - 1	COMP-BUR-1006-1008	241	0.0467	-	7470A	PPB	12 Mar 2021 11:54:14	U	SMPL
M1619-02DUP - 1	COMP-BUR-1006-1008	261	0.0515	-	7470A	PPB	12 Mar 2021 11:56:29	U	SMPL
M1619-02MS - 1	COMP-BUR-1006-1008	15772	3.7642	-	7470A	PPB	12 Mar 2021 11:58:44	U	SMPL
M1619-02MSD - 1	COMP-BUR-1006-1008	16943	4.0445	-	7470A	PPB	12 Mar 2021 12:01:00	U	SMPL
M1619-08 - 1	30624	757	0.1702	-	7470A	PPB	12 Mar 2021 12:03:16	U	SMPL
PB135119TB - 1	PB135093TB	220	0.0416	-	7470A	PPB	12 Mar 2021 12:05:32	U	SMPL
PB135120TB - 1	PB135103TB	362	0.0756	-	7470A	PPB	12 Mar 2021 12:07:49	U	SMPL
CCV14 - 1	CCV14	20986	5.0122	-	7470A	PPB	12 Mar 2021 12:10:05	U	SMPL
CCB14 - 1	CCB14	119	0.0175	-	7470A	PPB	12 Mar 2021 12:12:21	U	SMPL
M1565-11LX5 - 1		80	0.0081	-	7470A	PPB	12 Mar 2021 12:14:36	U	SMPL
M1565-11A - 1		15131	3.6108	-	7470A	PPB	12 Mar 2021 12:16:51	U	SMPL
M1619-02LX5 - 1		46	-0.0000	-	7470A	PPB	12 Mar 2021 12:19:07	U	SMPL
M1619-02A - 1		15267	3.6433	-	7470A	PPB	12 Mar 2021 12:21:22	U	SMPL
CCV15 - 1	CCV15	21244	5.0740	-	7470A	PPB	12 Mar 2021 12:23:38	U	SMPL
CCB15 - 1	CCB15	79	0.0079	-	7470A	PPB	12 Mar 2021 12:25:53	U	SMPL