

LB113554

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

3/17/2021 15:39

Test: Phenolics-

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	0.936	0.0	0.102	
ICB1	-0.001	0.0	0.006	
CCV1	0.942	0.0	0.102	
CCB1	-0.000	0.0	0.006	
PB135101BS	0.941	0.0	0.102	
PB135101BL	-0.003	0.0	0.006	
M1677-03	-0.000	0.0	0.006	
M1677-03DUP	-0.001	0.0	0.006	
M1677-03MS	0.912	0.0	0.099	
M1677-03MSD	0.894	0.0	0.097	
M1458-12	0.018	0.0	0.008	
CCV2	0.958	0.0	0.104	
CCB2	-0.005	0.0	0.006	

N	13
Mean	0.430
SD	0.4825
CV%	112.22

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 17 14:13:02 2021

Wed Mar 17 15:37:13 2021

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Phenolics-	P	-0.003	mg/l	3/17/2021 14:13:02	
0.05PPM	A	Phenolics-	P	0.0511	mg/l	3/17/2021 14:13:03	
0.1PPM	A	Phenolics-	P	0.1046	mg/l	3/17/2021 14:13:04	
0.25PPM	A	Phenolics-	P	0.2453	mg/l	3/17/2021 14:13:05	
0.50PPM	A	Phenolics-	P	0.5034	mg/l	3/17/2021 14:13:06	
1.0PPM	A	Phenolics-	P	0.9979	mg/l	3/17/2021 14:13:07	
2.0PPM	A	Phenolics-	P	2.0005	mg/l	3/17/2021 14:13:08	
ICV1	S	Phenolics-	P	0.9357	mg/l	3/17/2021 15:00:04	
ICB1	S	Phenolics-	P	-0.0013	mg/l	3/17/2021 15:00:06	
CCV1	S	Phenolics-	P	0.9417	mg/l	3/17/2021 15:00:09	
CCB1	S	Phenolics-	P	-0.0003	mg/l	3/17/2021 15:00:10	
PB135101BS	S	Phenolics-	P	0.9408	mg/l	3/17/2021 15:00:13	
PB135101BL	S	Phenolics-	P	-0.0029	mg/l	3/17/2021 15:00:15	
M1677-03	S	Phenolics-	P	-0.0003	mg/l	3/17/2021 15:10:12	
M1677-03DUP	S	Phenolics-	P	-0.0012	mg/l	3/17/2021 15:10:13	
M1677-03MS	S	Phenolics-	P	0.912	mg/l	3/17/2021 15:10:14	
M1677-03MSD	S	Phenolics-	P	0.8943	mg/l	3/17/2021 15:10:15	
M1458-12	S	Phenolics-	P	0.0178	mg/l	3/17/2021 15:37:03	
CCV2	S	Phenolics-	P	0.9584	mg/l	3/17/2021 15:37:09	
CCB2	S	Phenolics-	P	-0.0047	mg/l	3/17/2021 15:37:10	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

3/17/2021 14:25

Reviewed by : AM Instrument ID : Konelab


Test Phenolics-

Accepted 3/17/2021 14:25

Factor 9.78
Bias 0.006

Coeff. of det. 0.999978

Errors

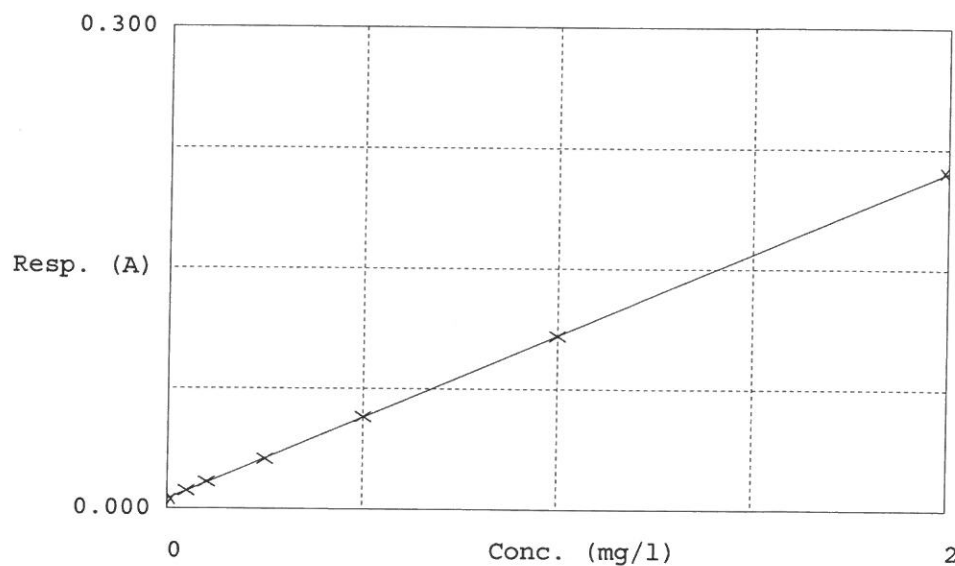

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.006	-0.0030	0.0000	
2	Phenol-2	0.011	0.0511	0.0500	
3	Phenol-2	0.017	0.1046	0.1000	
4	Phenol-2	0.031	0.2453	0.2500	
5	Phenol-2	0.058	0.5034	0.5000	
6	Phenol-2	0.108	0.9979	1.0000	
7	Phenol-2	0.211	2.0005	2.0000	

1% DI

1252100

3/17/2021
AM