

LB113589


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

40131

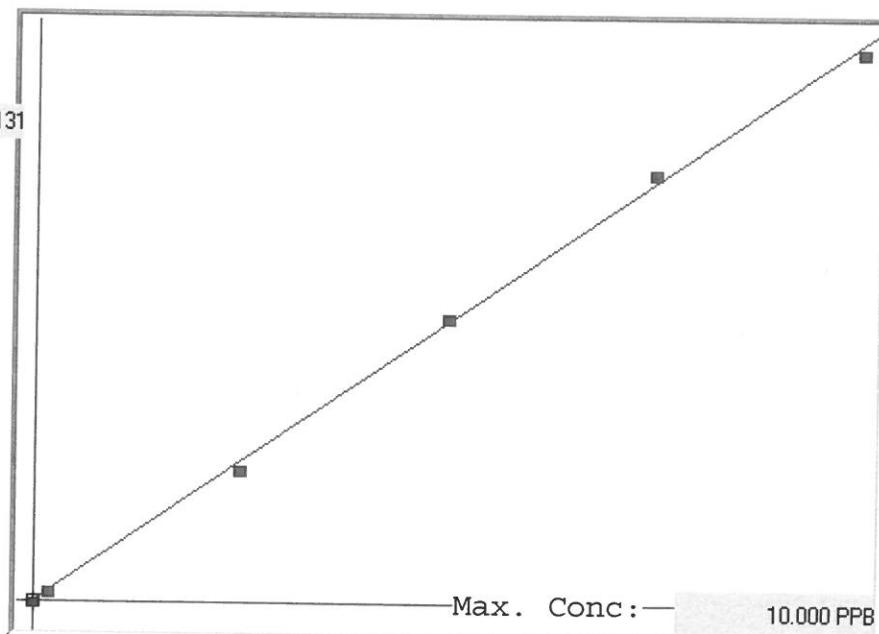

A= 0.0000e+000

B= 2.4553e-004

C= -2.8386e-003

Rho= 0.9995501

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.014	0.014	68	0.000	68					0/0
0.2	0.200	0.197	-0.003	814	0.0 %	814					-2
2.5	2.500	2.382	-0.118	9715	0.0 %	9715					-5
5.0	5.000	5.082	0.082	20710	0.0 %	20710					2
7.5	7.500	7.674	0.174	31268	0.0 %	31268					2
10.0	10.000	9.850	-0.150	40131	0.0 %	40131					-2

LB113589 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 19 Mar 2021 11:16:01						
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date		Type	Type
0.0 - 1	50	68	-	0.0000	7470A	PPB	19 Mar 2021	11:20:10	S	Std
0.2 - 1	50.2	814	-	0.2000	7470A	PPB	19 Mar 2021	11:22:27	S	Std
2.5 - 1	52.5	9715	-	2.5000	7470A	PPB	19 Mar 2021	11:24:44	S	Std
5.0 - 1	55	20710	-	5.0000	7470A	PPB	19 Mar 2021	11:27:01	S	Std
7.5 - 1	57.5	31268	-	7.5000	7470A	PPB	19 Mar 2021	11:29:17	S	Std
10.0 - 1	510	40131	-	10.0000	7470A	PPB	19 Mar 2021	11:34:05	S	Std
ICV43 - 1	ICV43	15612	3.8303	-	7470A	PPB	19 Mar 2021	11:36:44	U	SMPL
ICB43 - 1	ICB43	0	-0.0028	-	7470A	PPB	19 Mar 2021	11:38:58	U	SMPL
CCV45 - 1	CCV45	20872	5.1218	-	7470A	PPB	19 Mar 2021	11:41:13	U	SMPL
CCB45 - 1	CCB45	-7	-0.0046	-	7470A	PPB	19 Mar 2021	11:43:28	U	SMPL
CRA - 1	CRA	801	0.1938	-	7470A	PPB	19 Mar 2021	11:45:43	U	SMPL
HighStd - 1	HighStd	40102	9.8433	-	7470A	PPB	19 Mar 2021	11:47:58	U	SMPL
ChkStd - 1	ChkStd	29112	7.1449	-	7470A	PPB	19 Mar 2021	11:50:13	U	SMPL
PB135241BL - 1	PBW	-51	-0.0154	-	7470A	PPB	19 Mar 2021	11:52:29	U	SMPL
PB135241BS - 1	LCSW	15213	3.7324	-	7470A	PPB	19 Mar 2021	11:54:45	U	SMPL
M1682-03 - 1	SP-MANHOLE	18	0.0016	-	7470A	PPB	19 Mar 2021	11:57:01	U	SMPL
M1682-03DUP - 1	SP-MANHOLEDUP	45	0.0082	-	7470A	PPB	19 Mar 2021	11:59:18	U	SMPL
M1682-03MS - 1	SP-MANHOLEMS	15213	3.7324	-	7470A	PPB	19 Mar 2021	12:01:35	U	SMPL
M1682-03MSD - 1	SP-MANHOLEMSD	15436	3.7871	-	7470A	PPB	19 Mar 2021	12:03:51	U	SMPL
M1687-01 - 1	AUD-1052-1053	-5	-0.0041	-	7470A	PPB	19 Mar 2021	12:06:07	U	SMPL
CCV46 - 1	CCV46	20919	5.1333	-	7470A	PPB	19 Mar 2021	12:08:22	U	SMPL
CCB46 - 1	CCB46	-8	-0.0048	-	7470A	PPB	19 Mar 2021	12:10:37	U	SMPL
M1706-03 - 1	COMP:P-1:P-2:P-3:P-4	29	0.0043	-	7470A	PPB	19 Mar 2021	12:12:52	U	SMPL
M1707-03 - 1	ELEVATOR-510-EL-167-157	31	0.0048	-	7470A	PPB	19 Mar 2021	12:15:07	U	SMPL
M1707-06 - 1	ELEVATOR-511-EL-167-162	47	0.0087	-	7470A	PPB	19 Mar 2021	12:17:22	U	SMPL
M1707-09 - 1	ELEVATOR-511-EL-162-157	37	0.0062	-	7470A	PPB	19 Mar 2021	12:19:38	U	SMPL
M1709-03 - 1	PSHQ-SOIL	51	0.0097	-	7470A	PPB	19 Mar 2021	12:21:54	U	SMPL
M1712-18 - 1	EXTERNAL-PAD-COMP	59	0.0116	-	7470A	PPB	19 Mar 2021	12:24:10	U	SMPL
M1712-20 - 1	RED-BRICK-COMP	71	0.0146	-	7470A	PPB	19 Mar 2021	12:26:26	U	SMPL
M1712-22 - 1	NEW-BLOCK-FLOOR-PAT	365	0.0868	-	7470A	PPB	19 Mar 2021	12:28:43	U	SMPL
M1712-24 - 1	YELLOW-WALL-COMP	80	0.0168	-	7470A	PPB	19 Mar 2021	12:31:00	U	SMPL
PB135241TB - 1	PB135214TB	61	0.0121	-	7470A	PPB	19 Mar 2021	12:33:15	U	SMPL
CCV47 - 1	CCV47	21259	5.2168	-	7470A	PPB	19 Mar 2021	12:35:30	U	SMPL
CCB47 - 1	CCB47	8	-0.0009	-	7470A	PPB	19 Mar 2021	12:37:46	U	SMPL
M1682-03LX5 - 1		49	0.0092	-	7470A	PPB	19 Mar 2021	12:40:01	U	SMPL
M1682-03A - 1		15765	3.8679	-	7470A	PPB	19 Mar 2021	12:42:17	U	SMPL
CCV48 - 1	CCV48	20869	5.1211	-	7470A	PPB	19 Mar 2021	12:44:32	U	SMPL
CCB48 - 1	CCB48	2	-0.0023	-	7470A	PPB	19 Mar 2021	12:46:47	U	SMPL