


LB113623

7471B

INSTRUMENT ID: CV1

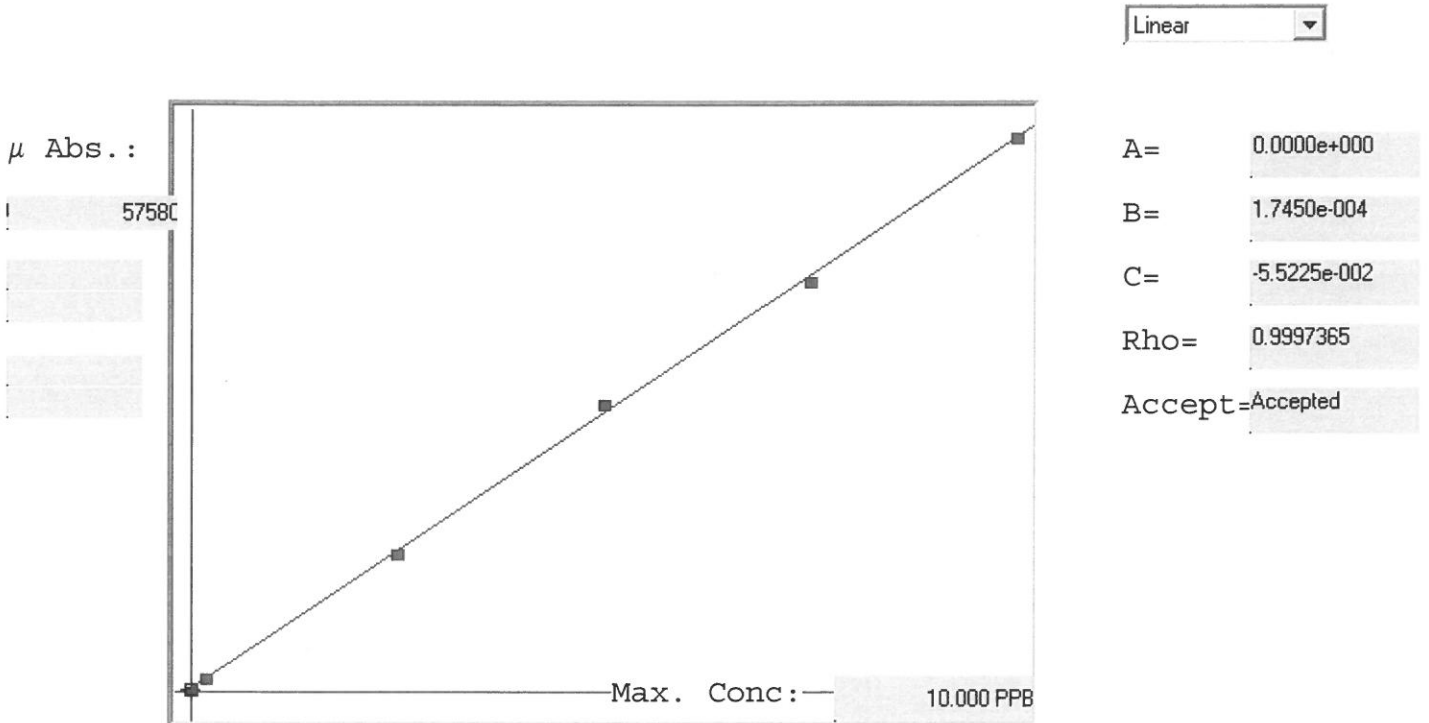

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.019	-0.019	205	0.000	205					-3
0.2	0.200	0.194	-0.006	1426	0.0 %	1426					-2
2.5	2.500	2.455	-0.045	14387	0.0 %	14387					4
5.0	5.000	5.176	0.176	29979	0.0 %	29979					-1
7.5	7.500	7.402	-0.098	42736	0.0 %	42736					0
10.0	10.000	9.992	-0.008	57580	0.0 %	57580					

LB113623 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 22 Mar 2021 15:05:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	205	-	0.00007471B	PPB		22 Mar 2021 15:06:33	S	Std
0.2 - 1	50.2	1426	-	0.20007471B	PPB		22 Mar 2021 15:08:50	S	Std
2.5 - 1	52.5	14387	-	2.50007471B	PPB		22 Mar 2021 15:11:07	S	Std
5.0 - 1	55	29979	-	5.00007471B	PPB		22 Mar 2021 15:13:24	S	Std
7.5 - 1	57.5	42736	-	7.50007471B	PPB		22 Mar 2021 15:15:40	S	Std
10.0 - 1	510	57580	-	10.00007471B	PPB		22 Mar 2021 15:17:56	S	Std
ICV46 - 1	ICV46	22613	3.8907	-7471B	PPB		22 Mar 2021 15:20:46	U	SMPL
ICB46 - 1	ICB46	238	-0.0137	-7471B	PPB		22 Mar 2021 15:23:00	U	SMPL
CCV56 - 1	CCV56	29894	5.1612	-7471B	PPB		22 Mar 2021 15:25:15	U	SMPL
CCB56 - 1	CCB56	226	-0.0158	-7471B	PPB		22 Mar 2021 15:27:30	U	SMPL
CRA - 1	CRA	1397	0.1885	-7471B	PPB		22 Mar 2021 15:29:45	U	SMPL
HighStd - 1	HighStd	57145	9.9165	-7471B	PPB		22 Mar 2021 15:32:00	U	SMPL
ChkStd - 1	ChkStd	40616	7.0322	-7471B	PPB		22 Mar 2021 15:34:15	U	SMPL
PB135277BL - 1	PB135277BL	128	-0.0329	-7471B	PPB		22 Mar 2021 15:36:32	U	SMPL
PB135277BS - 1	PB135277BS	21463	3.6900	-7471B	PPB		22 Mar 2021 15:38:48	U	SMPL
M1746-07 - 1	COMP-1	3584	0.5702	-7471B	PPB		22 Mar 2021 15:41:04	U	SMPL
M1746-07DUP - 1	COMP-1DUP	3815	0.6105	-7471B	PPB		22 Mar 2021 15:46:08	U	SMPL
M1746-07MS - 1	COMP-1MS	25561	4.4051	-7471B	PPB		22 Mar 2021 15:48:25	U	SMPL
M1746-07MSD - 1	COMP-1MSD	26631	4.5918	-7471B	PPB		22 Mar 2021 15:50:42	U	SMPL
M1746-08 - 1	COMP-2	3577	0.5690	-7471B	PPB		22 Mar 2021 15:52:57	U	SMPL
CCV57 - 1	CCV57	29732	5.1330	-7471B	PPB		22 Mar 2021 15:55:12	U	SMPL
CCB57 - 1	CCB57	211	-0.0184	-7471B	PPB		22 Mar 2021 15:57:27	U	SMPL
M1746-09 - 1	COMP-3	2811	0.4353	-7471B	PPB		22 Mar 2021 15:59:42	U	SMPL
M1746-10 - 1	COMP-4	2186	0.3262	-7471B	PPB		22 Mar 2021 16:01:58	U	SMPL
M1749-01 - 1	FS-SB-15-11-13	8716	1.4657	-7471B	PPB		22 Mar 2021 16:04:13	U	SMPL
M1749-02 - 1	FS-SB-15-21-22	469	0.0266	-7471B	PPB		22 Mar 2021 16:06:29	U	SMPL
M1751-01 - 1	BU-03-031921	3391	0.5365	-7471B	PPB		22 Mar 2021 16:08:44	U	SMPL
M1756-01 - 1	HR-03-031921	1209	0.1557	-7471B	PPB		22 Mar 2021 16:11:00	U	SMPL
M1746-07LX5 - 1		875	0.0975	-7471B	PPB		22 Mar 2021 16:13:16	U	SMPL
M1746-07A - 1		26073	4.4945	-7471B	PPB		22 Mar 2021 16:15:33	U	SMPL
CCV58 - 1	CCV58	29439	5.0818	-7471B	PPB		22 Mar 2021 16:17:49	U	SMPL
CCB58 - 1	CCB58	220	-0.0168	-7471B	PPB		22 Mar 2021 16:20:05	U	SMPL