

LB113675

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

3/25/2021 16:21

Test: Phenolics-

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	0.963	0.0	0.106	
ICB1	-0.002	0.0	0.005	
CCV1	0.963	0.0	0.106	
CCB1	-0.005	0.0	0.004	
PB135317BL	-0.004	0.0	0.004	
PB135317BS	0.969	0.0	0.107	
M1763-01	-0.010	0.0	0.004	
M1763-01DUP	-0.014	0.0	0.003	
M1763-01MS	1.015	0.0	0.111	
M1763-01MSD	1.013	0.0	0.111	
CCV2	0.956	0.0	0.105	
CCB2	-0.008	0.0	0.004	

N	12
Mean	0.486
SD	0.5158
CV%	106.06

Aquakem v. 7.2AQ1

Results from time period:

Thu Mar 25 15:38:36 2021

Thu Mar 25 16:13:44 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Phenolics-	P	-0.0066	mg/l	3/25/2021 15:38:36	
0.05PPM	A	Phenolics-	P	0.056	mg/l	3/25/2021 15:38:37	
0.1PPM	A	Phenolics-	P	0.1042	mg/l	3/25/2021 15:38:38	
0.25PPM	A	Phenolics-	P	0.2504	mg/l	3/25/2021 15:38:39	
0.50PPM	A	Phenolics-	P	0.4987	mg/l	3/25/2021 15:38:40	
1.0PPM	A	Phenolics-	P	0.9948	mg/l	3/25/2021 15:38:41	
2.0PPM	A	Phenolics-	P	2.0025	mg/l	3/25/2021 15:38:42	
ICV1	S	Phenolics-	P	0.9634	mg/l	3/25/2021 16:06:52	
ICB1	S	Phenolics-	P	-0.0018	mg/l	3/25/2021 16:06:54	
CCV1	S	Phenolics-	P	0.9634	mg/l	3/25/2021 16:06:55	
CCB1	S	Phenolics-	P	-0.005	mg/l	3/25/2021 16:06:57	
PB135317BL	S	Phenolics-	P	-0.0043	mg/l	3/25/2021 16:06:59	
PB135317BS	S	Phenolics-	P	0.9692	mg/l	3/25/2021 16:07:00	
M1763-01	S	Phenolics-	P	-0.0096	mg/l	3/25/2021 16:07:01	
M1763-01DUP	S	Phenolics-	P	-0.0143	mg/l	3/25/2021 16:07:02	
M1763-01MS	S	Phenolics-	P	1.0148	mg/l	3/25/2021 16:13:37	
M1763-01MSD	S	Phenolics-	P	1.013	mg/l	3/25/2021 16:13:38	
CCV2	S	Phenolics-	P	0.9557	mg/l	3/25/2021 16:13:40	
CCB2	S	Phenolics-	P	-0.0081	mg/l	3/25/2021 16:13:41	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

3/25/2021 15:42

Test Phenolics-


Accepted 3/25/2021 15:42

Factor 9.527

Bias 0.005

Coeff. of det. 0.999958

Errors

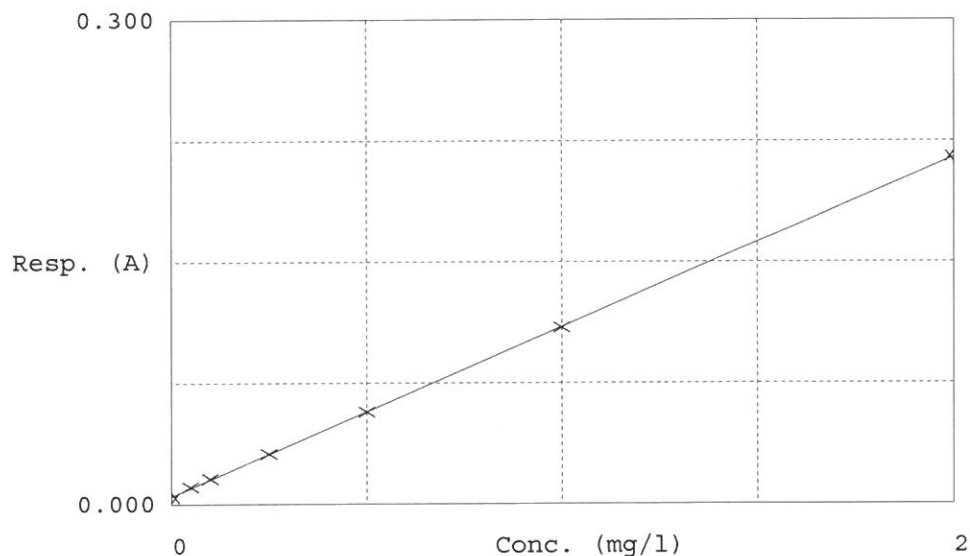

	Calibrator	Response	Calc. con.	Conc.	Errors	%D
1	0.00PPM	0.004	-0.0066	0.0000		
2	Phenol-2	0.011	0.0560	0.0500		
3	Phenol-2	0.016	0.1042	0.1000		
4	Phenol-2	0.031	0.2504	0.2500		
5	Phenol-2	0.057	0.4987	0.5000		
6	Phenol-2	0.109	0.9948	1.0000		
7	Phenol-2	0.215	2.0025	2.0000		

4
12
0
0
0
1
0

03/25/2021
AM