


LB113702

7471B

INSTRUMENT ID: CV2

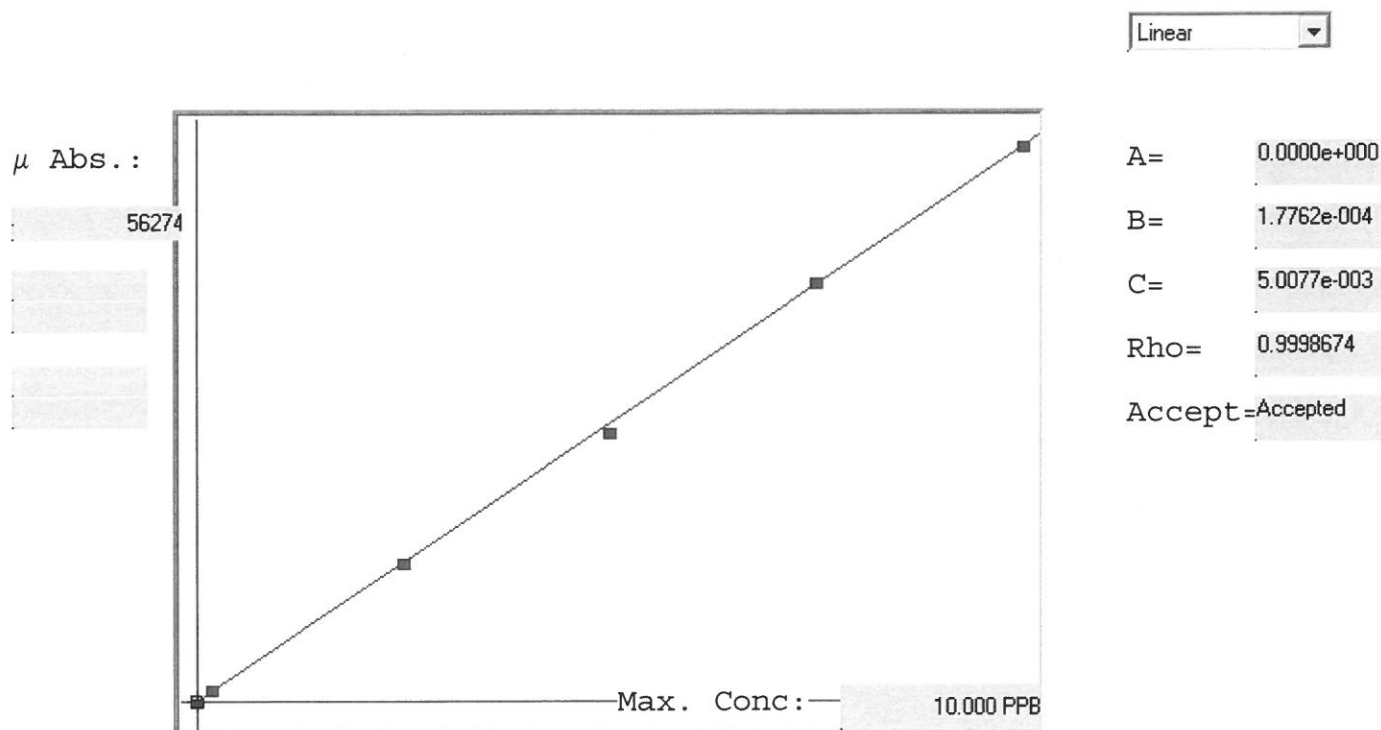

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	905
0.0	0.000	0.016	0.016	63	0.000	63					
0.2	0.200	0.224	0.024	1232	0.0 %	1232					
2.5	2.500	2.507	0.007	14085	0.0 %	14085					
5.0	5.000	4.877	-0.123	27431	0.0 %	27431					
7.5	7.500	7.576	0.076	42623	0.0 %	42623					
10.0	10.000	10.000	0.000	56274	0.0 %	56274					

905
12
0
-2
1
0

LB113702 INSTRUMENT ID : CV1

Method: 7471B	Operator: Admin	Date of Analysis: 26 Mar 2021 14:48:25							
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	56	63	-	0.0000	7471B	PPB	26 Mar 2021 14:50:41	S	Std
0.2 - 1	56-2	1232	-	0.2000	7471B	PPB	26 Mar 2021 14:52:58	S	Std
2.5 - 1	52.5	14085	-	2.5000	7471B	PPB	26 Mar 2021 14:55:15	S	Std
5.0 - 1	55	27431	-	5.0000	7471B	PPB	26 Mar 2021 14:57:32	S	Std
7.5 - 1	57.5	42623	-	7.5000	7471B	PPB	26 Mar 2021 14:59:48	S	Std
10.0 - 1	510	56274	-	10.0000	7471B	PPB	26 Mar 2021 15:02:03	S	Std
ICV55 - 1	ICV55	21734	3.8654	-	7471B	PPB	26 Mar 2021 15:07:16	U	SMPL
ICB55 - 1	ICB55	-26	0.0004	-	7471B	PPB	26 Mar 2021 15:09:31	U	SMPL
CCV91 - 1	CCV91	27030	4.8060	-	7471B	PPB	26 Mar 2021 15:11:46	U	SMPL
CCB91 - 1	CCB91	-31	-0.0005	-	7471B	PPB	26 Mar 2021 15:14:01	U	SMPL
CRA - 1	CRA	1196	0.2174	-	7471B	PPB	26 Mar 2021 15:16:15	U	SMPL
HighStd - 1	HighStd	55688	9.8962	-	7471B	PPB	26 Mar 2021 15:18:30	U	SMPL
ChkStd - 1	ChkStd	39683	7.0534	-	7471B	PPB	26 Mar 2021 15:20:45	U	SMPL
PB135385BL - 1	PBS	-85	-0.0101	-	7471B	PPB	26 Mar 2021 15:23:02	U	SMPL
PB135385BS - 1	LCSS	21971	3.9075	-	7471B	PPB	26 Mar 2021 15:25:17	U	SMPL
M1809-01 - 1	1-3-DRUM	6733	1.2009	-	7471B	PPB	26 Mar 2021 15:27:34	U	SMPL
M1810-01 - 1	600486548-BIN-1	3738	0.6689	-	7471B	PPB	26 Mar 2021 15:29:50	U	SMPL
M1811-01 - 1	031621-BIN-2	3153	0.5650	-	7471B	PPB	26 Mar 2021 15:32:06	U	SMPL
M1812-01 - 1	TP-1	630	0.1169	-	7471B	PPB	26 Mar 2021 15:34:24	U	SMPL
M1812-01DUP - 1	TP-1DUP	617	0.1146	-	7471B	PPB	26 Mar 2021 15:36:39	U	SMPL
CCV92 - 1	CCV92	26870	4.7776	-	7471B	PPB	26 Mar 2021 15:38:55	U	SMPL
CCB92 - 1	CCB92	-36	-0.0014	-	7471B	PPB	26 Mar 2021 15:41:09	U	SMPL
M1812-01MS - 1	TP-1MS	20982	3.7318	-	7471B	PPB	26 Mar 2021 15:43:25	U	SMPL
M1812-01MSD - 1	TP-1MSD	20995	3.7341	-	7471B	PPB	26 Mar 2021 15:45:40	U	SMPL
M1812-03 - 1	TP-2	958	0.1752	-	7471B	PPB	26 Mar 2021 15:47:56	U	SMPL
M1812-05 - 1	TP-3	1942	0.3499	-	7471B	PPB	26 Mar 2021 15:50:12	U	SMPL
M1813-01 - 1	L07	1767	0.3189	-	7471B	PPB	26 Mar 2021 15:52:27	U	SMPL
M1813-03 - 1	VNJ-236	740	0.1364	-	7471B	PPB	26 Mar 2021 15:54:43	U	SMPL
M1817-01 - 1	PHC-326FB-002	2604	0.4675	-	7471B	PPB	26 Mar 2021 15:56:59	U	SMPL
M1817-02 - 1	PHC-326FB-003	10324	1.8387	-	7471B	PPB	26 Mar 2021 15:59:16	U	SMPL
M1812-01LX5 - 1		80	0.0192	-	7471B	PPB	26 Mar 2021 16:01:32	U	SMPL
M1812-01A - 1		21400	3.8060	-	7471B	PPB	26 Mar 2021 16:03:48	U	SMPL
CCV93 - 1	CCV93	26951	4.7920	-	7471B	PPB	26 Mar 2021 16:06:03	U	SMPL
CCB93 - 1	CCB93	-37	-0.0016	-	7471B	PPB	26 Mar 2021 16:08:19	U	SMPL