

7470A


LB113717

INSTRUMENT ID: CV1

Linear

 μ Abs.:

38455

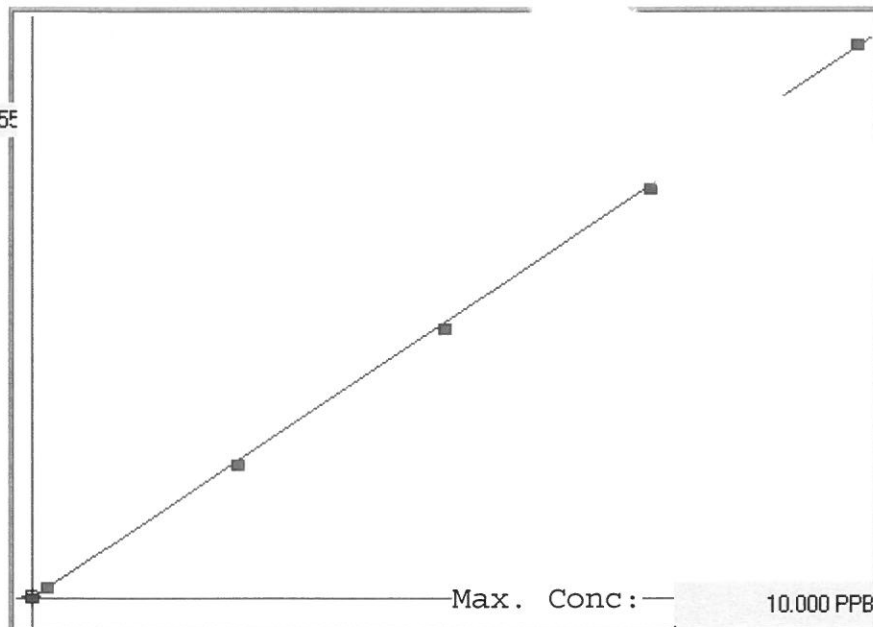

A= 0.0000e+000

B= 2.6160e-004

C= 9.3301e-003

= 0.9999050

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/o D
0.0	0.000	0.049	0.049	153	0.000	153					-
0.2	0.200	0.226	0.026	829	0.0 %	829					13
2.5	2.500	2.460	-0.040	9367	0.0 %	9367					-2
5.0	5.000	4.931	-0.069	18815	0.0 %	18815					-1
7.5	7.500	7.464	-0.036	28497	0.0 %	28497					0
10.0	10.000	10.069	0.069	38455	0.0 %	38455					1

LB113717 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 29 Mar 2021 12:32:09				Date	Type	Type
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units				
0.0 - 1		153	-	0.0000	7470A	PPB	29 Mar 2021	13:44:35	S	Std
0.2 - 1	50.2	829	-	0.2000	7470A	PPB	29 Mar 2021	13:46:51	S	Std
2.5 - 1	52.5	9367	-	2.5000	7470A	PPB	29 Mar 2021	13:49:09	S	Std
5.0 - 1	55	18815	-	5.0000	7470A	PPB	29 Mar 2021	13:51:25	S	Std
7.5 - 1	57.5	28497	-	7.5000	7470A	PPB	29 Mar 2021	13:53:42	S	Std
10.0 - 1	59.0	38455	-	10.0000	7470A	PPB	29 Mar 2021	14:01:55	S	Std
ICV56 - 1	ICV56	14363	3.7667	-	7470A	PPB	29 Mar 2021	14:04:39	U	SMPL
ICB56 - 1	ICB56	83	0.0310	-	7470A	PPB	29 Mar 2021	14:06:53	U	SMPL
CCV94 - 1	CCV94	17987	4.7147	-	7470A	PPB	29 Mar 2021	14:09:08	U	SMPL
CCB94 - 1	CCB94	84	0.0313	-	7470A	PPB	29 Mar 2021	14:11:23	U	SMPL
CRA - 1	CRA	835	0.2278	-	7470A	PPB	29 Mar 2021	14:13:38	U	SMPL
HighStd - 1	HighStd	38573	10.1001	-	7470A	PPB	29 Mar 2021	14:15:52	U	SMPL
ChkStd - 1	ChkStd	26724	7.0003	-	7470A	PPB	29 Mar 2021	14:18:08	U	SMPL
PB135409BL - 1	PBW	53	0.0232	-	7470A	PPB	29 Mar 2021	14:20:23	U	SMPL
PB135409BS - 1	LCSW	14849	3.8938	-	7470A	PPB	29 Mar 2021	14:22:38	U	SMPL
M1809-02 - 1	1-3-DRUM	74	0.0287	-	7470A	PPB	29 Mar 2021	14:24:55	U	SMPL
M1809-02DUP - 1	1-3-DRUMDUP	127	0.0426	-	7470A	PPB	29 Mar 2021	14:27:11	U	SMPL
M1809-02MS - 1	1-3-DRUMMS	14050	3.6848	-	7470A	PPB	29 Mar 2021	14:29:28	U	SMPL
M1809-02MSD - 1	1-3-DRUMMSD	15246	3.9977	-	7470A	PPB	29 Mar 2021	14:31:44	U	SMPL
M1817-03 - 1	PHC-326FB-002	21	0.0148	-	7470A	PPB	29 Mar 2021	14:33:59	U	SMPL
CCV95 - 1	CCV95	18469	4.8408	-	7470A	PPB	29 Mar 2021	14:36:15	U	SMPL
CCB95 - 1	CCB95	74	0.0287	-	7470A	PPB	29 Mar 2021	14:38:30	U	SMPL
M1817-04 - 1	PHC-326FB-003	274	0.0810	-	7470A	PPB	29 Mar 2021	14:40:45	U	SMPL
M1821-04 - 1	EL-509-STREET-LEVEL	120	0.0407	-	7470A	PPB	29 Mar 2021	14:43:00	U	SMPL
M1821-05 - 1	EL-510-STREET-LEVEL	138	0.0454	-	7470A	PPB	29 Mar 2021	14:45:16	U	SMPL
M1821-06 - 1	EL-511-STREET-LEVEL	120	0.0407	-	7470A	PPB	29 Mar 2021	14:47:31	U	SMPL
M1830-01 - 1	DRUM1-POLY	129	0.0431	-	7470A	PPB	29 Mar 2021	14:49:47	U	SMPL
M1830-02 - 1	DRUM1-PPE	132	0.0439	-	7470A	PPB	29 Mar 2021	14:52:03	U	SMPL
M1832-06 - 1	IG001	133	0.0441	-	7470A	PPB	29 Mar 2021	14:54:19	U	SMPL
M1832-07 - 1	IG002	135	0.0446	-	7470A	PPB	29 Mar 2021	14:56:36	U	SMPL
M1832-08 - 1	IG003	129	0.0431	-	7470A	PPB	29 Mar 2021	14:58:52	U	SMPL
M1832-09 - 1	IG004	147	0.0478	-	7470A	PPB	29 Mar 2021	15:01:08	U	SMPL
CCV96 - 1	CCV96	18835	4.9366	-	7470A	PPB	29 Mar 2021	15:03:23	U	SMPL
CCB96 - 1	CCB96	92	0.0334	-	7470A	PPB	29 Mar 2021	15:05:39	U	SMPL
M1832-10 - 1	IG005	135	0.0446	-	7470A	PPB	29 Mar 2021	15:07:54	U	SMPL
M1838-02 - 1	PHC-BEAPT-001	232	0.0700	-	7470A	PPB	29 Mar 2021	15:10:10	U	SMPL
PB135410BL - 1	PBW	87	0.0321	-	7470A	PPB	29 Mar 2021	15:12:25	U	SMPL
PB135410BS - 1	LCSW	14054	3.6859	-	7470A	PPB	29 Mar 2021	15:14:40	U	SMPL
M1825-01 - 1	FM5210	82	0.0308	-	7470A	PPB	29 Mar 2021	15:16:56	U	SMPL
M1825-01DUP - 1	FM5210DUP	139	0.0457	-	7470A	PPB	29 Mar 2021	15:19:12	U	SMPL
M1825-01MS - 1	FM5210MS	12872	3.3767	-	7470A	PPB	29 Mar 2021	15:21:29	U	SMPL
M1825-01MSD - 1	FM5210MSD	12665	3.3225	-	7470A	PPB	29 Mar 2021	15:23:46	U	SMPL
CCV97 - 1	CCV97	17777	4.6598	-	7470A	PPB	29 Mar 2021	15:26:03	U	SMPL
CCB97 - 1	CCB97	71	0.0279	-	7470A	PPB	29 Mar 2021	15:28:18	U	SMPL
PB135409TB - 1	PB135366TB	106	0.0371	-	7470A	PPB	29 Mar 2021	15:30:33	U	SMPL
M1809-02LX5 - 1		123	0.0415	-	7470A	PPB	29 Mar 2021	15:32:49	U	SMPL
M1809-02A - 1		15444	4.0495	-	7470A	PPB	29 Mar 2021	15:35:04	U	SMPL
M1825-01LX5 - 1		89	0.0326	-	7470A	PPB	29 Mar 2021	15:37:19	U	SMPL
M1825-01A - 1		14784	3.8768	-	7470A	PPB	29 Mar 2021	15:39:35	U	SMPL
CCV98 - 1	CCV98	18967	4.9711	-	7470A	PPB	29 Mar 2021	15:41:50	U	SMPL
CCB98 - 1	CCB98	77	0.0295	-	7470A	PPB	29 Mar 2021	15:44:06	U	SMPL