


LB118743

245.1

INSTRUMENT ID: CV1

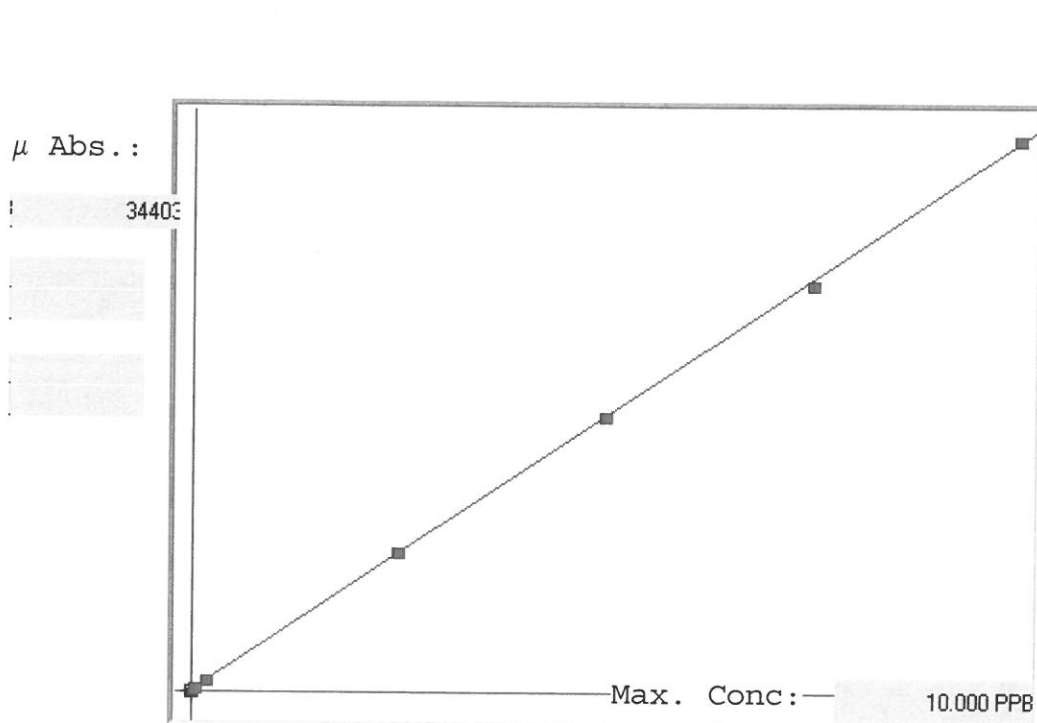

Linear

A= 0.0000e+000

B= 2.9271e-004

C= -2.1983e-002

Rho= 0.9999397

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.000	-0.000	75	0.000	75					
0.05	0.050	0.048	-0.002	239	0.0 %	239	0				-4
0.2	0.200	0.188	-0.012	719	0.0 %	719					-6
2.5	2.500	2.541	0.041	8756	0.0 %	8756					2
5.0	5.000	5.011	0.011	17193	0.0 %	17193					0
7.5	7.500	7.414	-0.086	25404	0.0 %	25404					-1
10.0	10.000	10.048	0.048	34403	0.0 %	34403					0

LB113743 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 30 Mar 2021 11:18:30

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	75	-	0.0000	245.1	PPB	30 Mar 2021 11:40:13	S	Std
0.05 - 1	50.05	239	-	0.0500	245.1	PPB	30 Mar 2021 11:42:30	S	Std
0.2 - 1	50.2	719	-	0.2000	245.1	PPB	30 Mar 2021 11:44:47	S	Std
2.5 - 1	52.5	8756	-	2.5000	245.1	PPB	30 Mar 2021 11:47:03	S	Std
5.0 - 1	55	17193	-	5.0000	245.1	PPB	30 Mar 2021 11:49:19	S	Std
7.5 - 1	57.5	25404	-	7.5000	245.1	PPB	30 Mar 2021 11:51:35	S	Std
10.0 - 1	510	34403	-	10.0000	245.1	PPB	30 Mar 2021 11:56:24	S	Std
ICV58 - 1	ICV58	13619	3.9644	-245.1		PPB	30 Mar 2021 11:59:08	U	SMPL
ICB58 - 1	ICB58	-15	-0.0264	-245.1		PPB	30 Mar 2021 12:01:23	U	SMPL
CCV05 - 1	CCV05	17422	5.0776	-245.1		PPB	30 Mar 2021 12:03:37	U	SMPL
CCB05 - 1	CCB05	-20	-0.0278	-245.1		PPB	30 Mar 2021 12:05:52	U	SMPL
CRA - 1	CRA	219	0.0421	-245.1		PPB	30 Mar 2021 12:08:07	U	SMPL
HighStd - 1	HighStd	34106	9.9611	-245.1		PPB	30 Mar 2021 12:10:21	U	SMPL
ChkStd - 1	ChkStd	25428	7.4210	-245.1		PPB	30 Mar 2021 12:12:36	U	SMPL
PB135439BL - 1	PBW	-55	-0.0381	-245.1		PPB	30 Mar 2021 12:14:52	U	SMPL
PB135439BS - 1	LCSW	14865	4.3291	-245.1		PPB	30 Mar 2021 12:17:08	U	SMPL
M1695-01 - 1	EFFLUENT-DAY1-METALS	450	0.1097	-245.1		PPB	30 Mar 2021 12:19:24	U	SMPL
M1763-03 - 1	EL-509-WATER-SAMPLE	157	0.0240	-245.1		PPB	30 Mar 2021 12:21:41	U	SMPL
M1863-03 - 1	HP-640	67	-0.0024	-245.1		PPB	30 Mar 2021 12:23:57	U	SMPL
M1863-03DUP - 1	HP-640DUP	91	0.0047	-245.1		PPB	30 Mar 2021 12:26:14	U	SMPL
M1863-03MS - 1	HP-640MS	13157	3.8292	-245.1		PPB	30 Mar 2021 12:28:29	U	SMPL
CCV06 - 1	CCV06	16235	4.7301	-245.1		PPB	30 Mar 2021 12:30:45	U	SMPL
CCB06 - 1	CCB06	-35	-0.0322	-245.1		PPB	30 Mar 2021 12:33:00	U	SMPL
M1863-03MSD - 1	HP-640MSD	12932	3.7633	-245.1		PPB	30 Mar 2021 12:35:15	U	SMPL
M1863-03LX5 - 1		-14	-0.0261	-245.1		PPB	30 Mar 2021 12:37:31	U	SMPL
M1863-03A - 1		12836	3.7352	-245.1		PPB	30 Mar 2021 12:39:46	U	SMPL
CCV07 - 1	CCV07	16739	4.8777	-245.1		PPB	30 Mar 2021 12:42:02	U	SMPL
CCB07 - 1	CCB07	-76	-0.0442	-245.1		PPB	30 Mar 2021 12:44:17	U	SMPL