


LB113769

7470A

INSTRUMENT ID: CV2

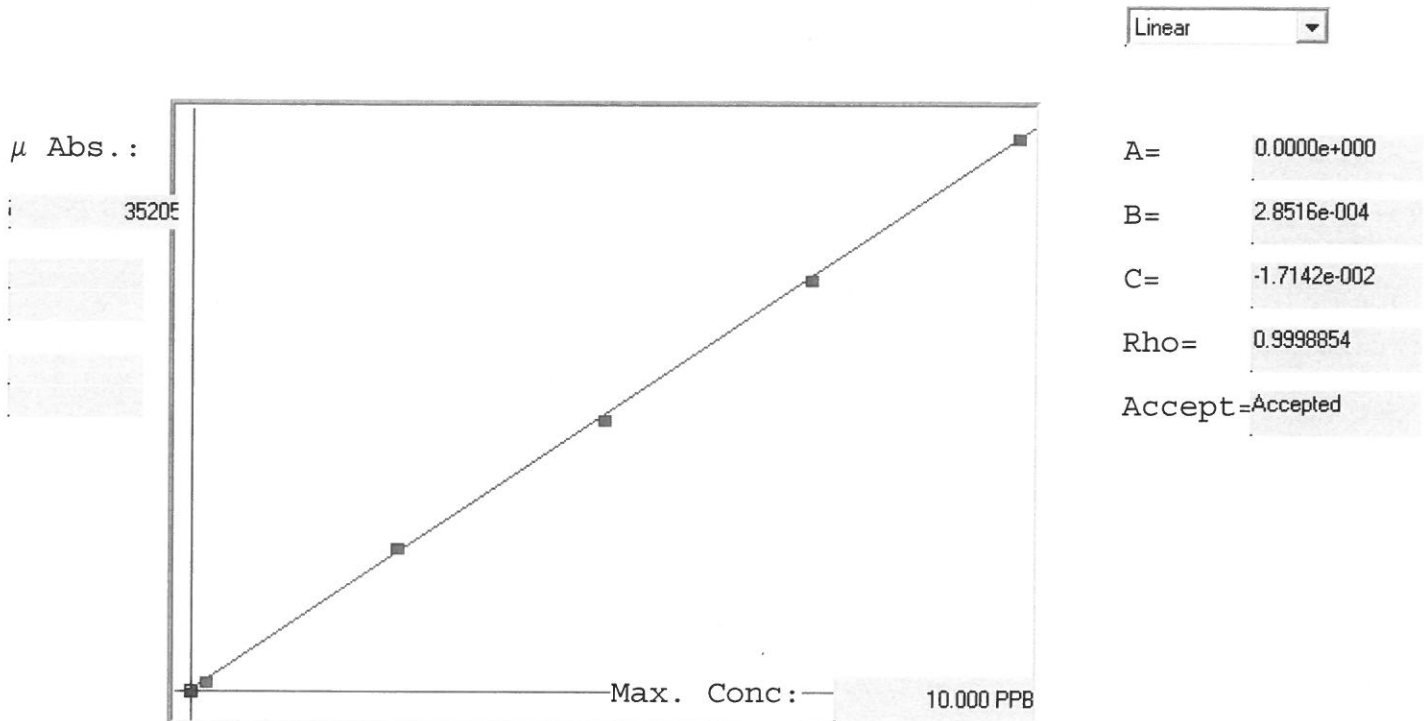

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	-0.013	-0.013	16	0.000	16					
0.2	0.200	0.174	-0.026	671	0.0 %	671					
2.5	2.500	2.608	0.108	9206	0.0 %	9206					
5.0	5.000	4.926	-0.074	17336	0.0 %	17336					
7.5	7.500	7.482	-0.018	26298	0.0 %	26298					
10.0	10.000	10.022	0.022	35205	0.0 %	35205					

0/01

-13

4

-1

0

0

LB113769 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 31 Mar 2021 14:00:20

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	16	-	0.0000	7470A	PPB	31 Mar 2021 14:06:39	S	Std
0.2 - 1	50.2	671	-	0.2000	7470A	PPB	31 Mar 2021 14:08:55	S	Std
2.5 - 1	52.5	9206	-	2.5000	7470A	PPB	31 Mar 2021 14:11:12	S	Std
5.0 - 1	55	17336	-	5.0000	7470A	PPB	31 Mar 2021 14:13:28	S	Std
7.5 - 1	57.5	26298	-	7.5000	7470A	PPB	31 Mar 2021 14:18:24	S	Std
10.0 - 1	510	35205	-	10.0000	7470A	PPB	31 Mar 2021 14:26:04	S	Std
ICV62 - 1	ICV62	13563	3.8505	-7470A	PPB	31 Mar 2021 14:28:49	U	SMPL	
ICB62 - 1	ICB62	-118	-0.0508	-7470A	PPB	31 Mar 2021 14:33:39	U	SMPL	
CCV17 - 1	CCV17	18029	5.1240	-7470A	PPB	31 Mar 2021 14:38:50	U	SMPL	
CCB17 - 1	CCB17	-70	-0.0371	-7470A	PPB	31 Mar 2021 14:43:36	U	SMPL	
CRA - 1	CRA	616	0.1585	-7470A	PPB	31 Mar 2021 14:45:51	U	SMPL	
HighStd - 1	HighStd	34709	9.8805	-7470A	PPB	31 Mar 2021 14:48:05	U	SMPL	
ChkStd - 1	ChkStd	24939	7.0945	-7470A	PPB	31 Mar 2021 14:50:21	U	SMPL	
PB135467BL - 1	PBW	-104	-0.0468	-7470A	PPB	31 Mar 2021 14:55:10	U	SMPL	
PB135467BS - 1	LCSW	14939	4.2429	-7470A	PPB	31 Mar 2021 14:57:26	U	SMPL	
M1864-01 - 1	MMR-SP	-262	-0.0919	-7470A	PPB	31 Mar 2021 14:59:42	U	SMPL	
M1872-03 - 1	SP-GIS	-68	-0.0365	-7470A	PPB	31 Mar 2021 15:01:59	U	SMPL	
M1872-03DUP - 1	SP-GISDUP	-27	-0.0248	-7470A	PPB	31 Mar 2021 15:04:16	U	SMPL	
M1872-03MS - 1	SP-GISMS	15104	4.2899	-7470A	PPB	31 Mar 2021 15:06:33	U	SMPL	
M1872-03MSD - 1	SP-GISMSD	13590	3.8582	-7470A	PPB	31 Mar 2021 15:08:48	U	SMPL	
CCV18 - 1	CCV18	16592	4.7142	-7470A	PPB	31 Mar 2021 15:11:04	U	SMPL	
CCB18 - 1	CCB18	-80	-0.0400	-7470A	PPB	31 Mar 2021 15:16:01	U	SMPL	
PB135468BL - 1	PBW	1	-0.0169	-7470A	PPB	31 Mar 2021 15:18:16	U	SMPL	
PB135468BS - 1	LCSW	14166	4.0224	-7470A	PPB	31 Mar 2021 15:20:31	U	SMPL	
M1835-02 - 1	ASR7	881	0.2341	-7470A	PPB	31 Mar 2021 15:33:37	U	SMPL	
M1835-02DUP - 1	ASR7DUP	874	0.2321	-7470A	PPB	31 Mar 2021 15:35:52	U	SMPL	
M1835-02MS - 1	ASR7MS	15480	4.3971	-7470A	PPB	31 Mar 2021 15:38:08	U	SMPL	
M1835-02MSD - 1	ASR7MSD	15234	4.3270	-7470A	PPB	31 Mar 2021 15:40:24	U	SMPL	
M1835-04 - 1	ASR5	115	0.0157	-7470A	PPB	31 Mar 2021 15:42:41	U	SMPL	
M1835-06 - 1	ASR6	350	0.0827	-7470A	PPB	31 Mar 2021 15:44:58	U	SMPL	
M1835-10 - 1	ASR7	225	0.0470	-7470A	PPB	31 Mar 2021 15:47:14	U	SMPL	
CCV19 - 1	CCV19	17982	5.1106	-7470A	PPB	31 Mar 2021 15:49:29	U	SMPL	
CCB19 - 1	CCB19	-67	-0.0362	-7470A	PPB	31 Mar 2021 15:51:44	U	SMPL	
M1835-11 - 1	ASR5	9	-0.0146	-7470A	PPB	31 Mar 2021 15:54:00	U	SMPL	
M1835-12 - 1	ASR6	77	0.0048	-7470A	PPB	31 Mar 2021 15:56:15	U	SMPL	
M1873-09 - 1	TOTE-COMP	1012	0.2714	-7470A	PPB	31 Mar 2021 15:58:31	U	SMPL	
PB135467TB - 1	PB35443TB	-10	-0.0200	-7470A	PPB	31 Mar 2021 16:00:46	U	SMPL	
M1872-03LX5 - 1		9	-0.0146	-7470A	PPB	31 Mar 2021 16:03:01	U	SMPL	
M1872-03A - 1		14519	4.1231	-7470A	PPB	31 Mar 2021 16:05:18	U	SMPL	
M1835-02LX5 - 1		138	0.0222	-7470A	PPB	31 Mar 2021 16:07:34	U	SMPL	
M1835-02A - 1		15724	4.4667	-7470A	PPB	31 Mar 2021 16:09:50	U	SMPL	
M1764-06 - 1	COMP-OILY-WATER	452	0.1118	-7470A	PPB	31 Mar 2021 16:12:07	U	SMPL	
CCV20 - 1	CCV20	17608	5.0040	-7470A	PPB	31 Mar 2021 16:14:23	U	SMPL	
CCB20 - 1	CCB20	-69	-0.0368	-7470A	PPB	31 Mar 2021 16:16:39	U	SMPL	