

LB113849

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

4/6/2021 16:35

Test: Phenolics-

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	1.003	0.0	0.114	
ICB1	-0.002	0.0	0.005	
CCV1	0.998	0.0	0.113	
CCB1	-0.003	0.0	0.005	
PB135579BL	-0.003	0.0	0.005	
PB135579BS	0.995	0.0	0.113	
M1951-04	-0.000	0.0	0.005	
M1951-05	-0.001	0.0	0.005	
M1951-01	-0.005	0.0	0.005	
M1951-01DUP	-0.006	0.0	0.004	
M1951-02MS	0.868	0.0	0.099	
M1951-03MSD	0.878	0.0	0.100	
CCV2	1.006	0.0	0.114	
CCB2	-0.004	0.0	0.005	

N	14
Mean	0.409
SD	0.4954
CV%	121.16

Aquakem v. 7.2AQ1

Results from time period:

Tue Apr 06 15:39:16 2021

Tue Apr 06 16:34:22 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Phenolics-	P	-0.0007	mg/l	4/6/2021 15:39:16	
0.05PPM	A	Phenolics-	P	0.0495	mg/l	4/6/2021 15:39:17	
0.1PPM	A	Phenolics-	P	0.0996	mg/l	4/6/2021 15:39:18	
0.25PPM	A	Phenolics-	P	0.2525	mg/l	4/6/2021 15:39:19	
0.50PPM	A	Phenolics-	P	0.4955	mg/l	4/6/2021 15:39:20	
1.0PPM	A	Phenolics-	P	1.0056	mg/l	4/6/2021 15:39:21	
2.0PPM	A	Phenolics-	P	1.998	mg/l	4/6/2021 15:39:22	
ICV1	S	Phenolics-	P	1.0032	mg/l	4/6/2021 16:07:11	
ICB1	S	Phenolics-	P	-0.0016	mg/l	4/6/2021 16:07:12	
CCV1	S	Phenolics-	P	0.9983	mg/l	4/6/2021 16:07:15	
CCB1	S	Phenolics-	P	-0.0034	mg/l	4/6/2021 16:07:16	
PB135579BL	S	Phenolics-	P	-0.0034	mg/l	4/6/2021 16:07:18	
PB135579BS	S	Phenolics-	P	0.9955	mg/l	4/6/2021 16:07:19	
M1951-04	S	Phenolics-	P	0	mg/l	4/6/2021 16:17:16	
M1951-05	S	Phenolics-	P	-0.0012	mg/l	4/6/2021 16:17:17	
M1951-01	S	Phenolics-	P	-0.0048	mg/l	4/6/2021 16:28:45	
M1951-01DUP	S	Phenolics-	P	-0.0065	mg/l	4/6/2021 16:31:40	
M1951-02MS	S	Phenolics-	P	0.8685	mg/l	4/6/2021 16:31:41	
M1951-03MSD	S	Phenolics-	P	0.878	mg/l	4/6/2021 16:31:42	
CCV2	S	Phenolics-	P	1.0056	mg/l	4/6/2021 16:34:21	
CCB2	S	Phenolics-	P	-0.0041	mg/l	4/6/2021 16:34:22	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

4/6/2021 15:40


Test Phenolics-

Accepted 4/6/2021 15:39

Factor 9.209
Bias 0.005

Coeff. of det. 0.999980

Errors

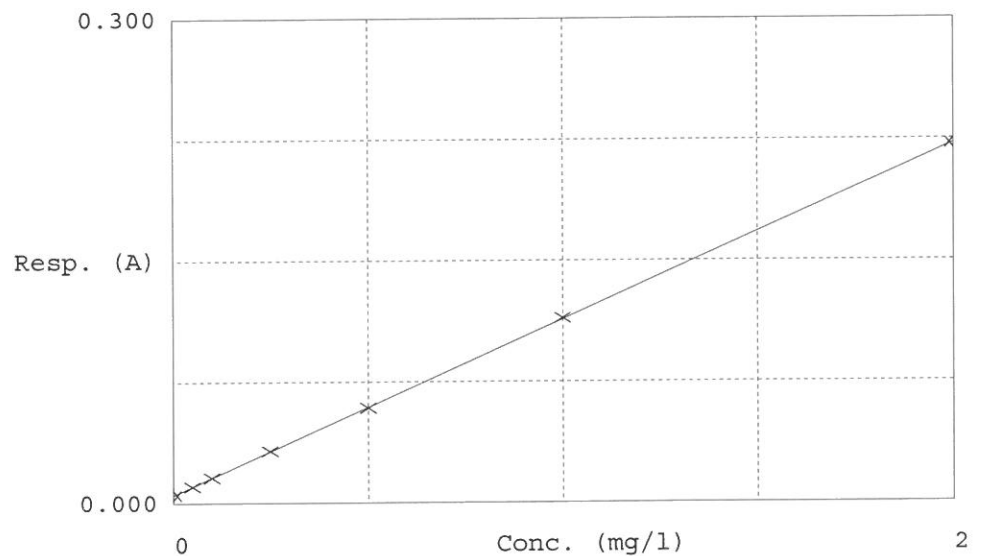

	Calibrator	Response	Calc. con.	Conc.	Errors	%D
1	0.00PPM	0.005	-0.0007	0.0000		1
2	Phenol-2	0.010	0.0495	0.0500		0
3	Phenol-2	0.016	0.0996	0.1000		1
4	Phenol-2	0.032	0.2525	0.2500		1
5	Phenol-2	0.059	0.4955	0.5000		0
6	Phenol-2	0.114	1.0056	1.0000		0
7	Phenol-2	0.222	1.9980	2.0000		0

04/06/2021
AM