

LB 113972


7470A

INSTRUMENT ID: LV1

Linear

μ Abs.:

38121

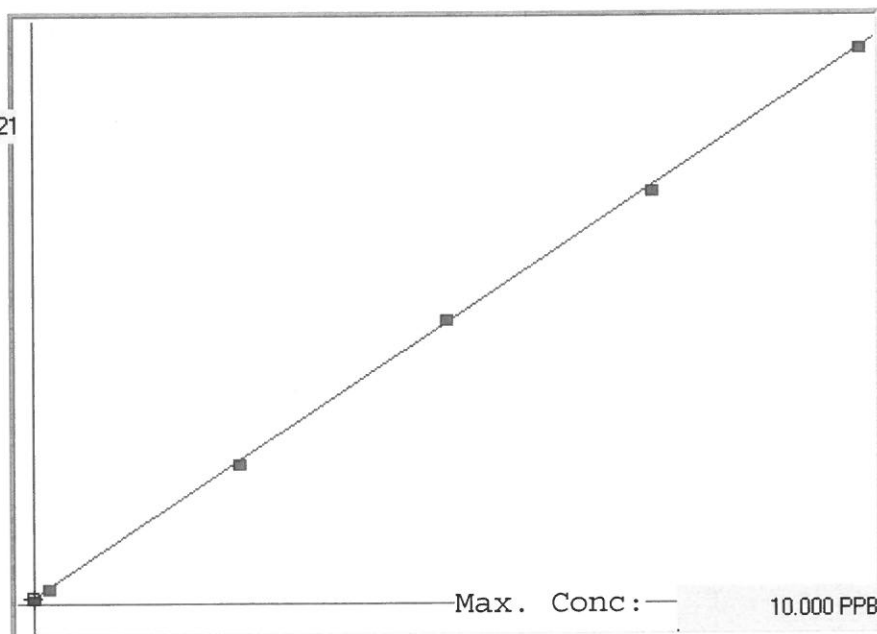

A= 0.0000e+000

B= 2.6525e-004

C= -1.0440e-001

Rho= 0.9999361

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.002	0.002	402	0.000	402					
0.2	0.200	0.195	-0.005	1129	0.0 %	1129					-3
2.5	2.500	2.469	-0.031	9703	0.0 %	9703					-1
5.0	5.000	5.080	0.080	19547	0.0 %	19547					2
7.5	7.500	7.446	-0.054	28464	0.0 %	28464					-1
10.0	10.000	10.007	0.007	38121	0.0 %	38121					0

LB113972 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Apr 2021 11:22:53

Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	402	-	0.0000	7470A	PPB	14 Apr 2021 11:36:49	S	Std
0.2 - 1	50.2	1129	-	0.2000	7470A	PPB	14 Apr 2021 11:39:06	S	Std
2.5 - 1	52.5	9703	-	2.5000	7470A	PPB	14 Apr 2021 11:41:23	S	Std
5.0 - 1	55	19547	-	5.0000	7470A	PPB	14 Apr 2021 11:43:39	S	Std
7.5 - 1	57.5	28464	-	7.5000	7470A	PPB	14 Apr 2021 11:45:55	S	Std
10.0 - 1	59	38121	-	10.0000	7470A	PPB	14 Apr 2021 11:50:46	S	Std
ICV85 - 1	ICV85	15431	3.9887	-	7470A	PPB	14 Apr 2021 11:53:29	U	SMPL
ICB85 - 1	ICB85	134	-0.0689	-	7470A	PPB	14 Apr 2021 11:55:44	U	SMPL
CCV01 - 1	CCV01	19964	5.1911	-	7470A	PPB	14 Apr 2021 11:57:59	U	SMPL
CCB01 - 1	CCB01	177	-0.0575	-	7470A	PPB	14 Apr 2021 12:00:14	U	SMPL
CRA - 1	CRA	1110	0.1900	-	7470A	PPB	14 Apr 2021 12:02:30	U	SMPL
HighStd - 1	HighStd	38550	10.1210	-	7470A	PPB	14 Apr 2021 12:04:45	U	SMPL
ChkStd - 1	ChkStd	25393	6.6311	-	7470A	PPB	14 Apr 2021 12:07:00	U	SMPL
PB135716BL - 1	PBW	416	0.0059	-	7470A	PPB	14 Apr 2021 12:11:49	U	SMPL
PB135716BS - 1	LCSW	15417	3.9850	-	7470A	PPB	14 Apr 2021 12:14:04	U	SMPL
M1982-03 - 1	WC-1	546	0.0404	-	7470A	PPB	14 Apr 2021 12:16:20	U	SMPL
M2008-03 - 1	NANUET-ST-041221	527	0.0354	-	7470A	PPB	14 Apr 2021 12:18:36	U	SMPL
M2012-01 - 1	MS-PC	367	-0.0071	-	7470A	PPB	14 Apr 2021 12:20:53	U	SMPL
M2016-06 - 1	DRUM-OIL	633	0.0635	-	7470A	PPB	14 Apr 2021 12:23:09	U	SMPL
M2019-02 - 1	149TH-ST-E1-101	219	-0.0463	-	7470A	PPB	14 Apr 2021 12:25:25	U	SMPL
CCV02 - 1	CCV02	18157	4.7118	-	7470A	PPB	14 Apr 2021 12:30:15	U	SMPL
CCB02 - 1	CCB02	158	-0.0625	-	7470A	PPB	14 Apr 2021 12:32:30	U	SMPL
M2019-02DUP - 1	149TH-ST-E1-101DUP	407	0.0036	-	7470A	PPB	14 Apr 2021 12:34:47	U	SMPL
M2019-02MS - 1	149TH-ST-E1-101MS	12780	3.2855	-	7470A	PPB	14 Apr 2021 12:37:01	U	SMPL
M2019-02MSD - 1	149TH-ST-E1-101MSD	14229	3.6699	-	7470A	PPB	14 Apr 2021 12:39:17	U	SMPL
PB135717BL - 1	PBW	320	-0.0195	-	7470A	PPB	14 Apr 2021 12:41:33	U	SMPL
PB135717BS - 1	LCSW	14175	3.6555	-	7470A	PPB	14 Apr 2021 12:43:48	U	SMPL
M2014-04 - 1	16128	447753	HIGH	-	7470A	PPB	14 Apr 2021 12:46:04	X	
M2014-04DUP - 1	16128DUP	438483	HIGH	-	7470A	PPB	14 Apr 2021 12:47:54	X	
M2014-04MS - 1	16128MS	443466	HIGH	-	7470A	PPB	14 Apr 2021 12:49:49	X	
M2014-04MSD - 1	16128MSD	441601	HIGH	-	7470A	PPB	14 Apr 2021 12:51:42	X	
CCV03 - 1	CCV03	18885	4.9049	-	7470A	PPB	14 Apr 2021 12:53:36	U	SMPL
CCB03 - 1	CCB03	176	-0.0577	-	7470A	PPB	14 Apr 2021 12:55:54	U	SMPL
PB135716TB - 1	PB135691TB	302	-0.0243	-	7470A	PPB	14 Apr 2021 13:00:49	U	SMPL
M2019-02LX5 - 1		338	-0.0147	-	7470A	PPB	14 Apr 2021 13:03:05	U	SMPL
M2019-02A - 1		13946	3.5948	-	7470A	PPB	14 Apr 2021 13:07:54	U	SMPL
M2014-04LX5 - 1		154472	40.8694	-	7470A	PPB	14 Apr 2021 13:10:09	U	SMPL
M2014-04A - 1		408715	HIGH	-	7470A	PPB	14 Apr 2021 13:12:25	X	
M2014-04DLX10 - 1		79700	21.0361	-	7470A	PPB	14 Apr 2021 13:14:17	U	SMPL
M2014-04DUPDLX10 - 1		81806	21.5947	-	7470A	PPB	14 Apr 2021 13:16:35	U	SMPL
M2014-04MSDLX10 - 1		78088	20.6085	-	7470A	PPB	14 Apr 2021 13:18:53	U	SMPL
M2014-04MSDDLX10 - 1		81722	21.5724	-	7470A	PPB	14 Apr 2021 13:21:11	U	SMPL
CCV04 - 1	CCV04	19519	5.0730	-	7470A	PPB	14 Apr 2021 13:23:30	U	SMPL
CCB04 - 1	CCB04	181	-0.0564	-	7470A	PPB	14 Apr 2021 13:25:47	U	SMPL
M2014-04LDL2X50 - 1		15476	4.0006	-	7470A	PPB	14 Apr 2021 13:28:02	U	SMPL
M2014-04ADL2X10 - 1		77408	20.4281	-	7470A	PPB	14 Apr 2021 13:30:17	U	SMPL
M2014-04DL2X50 - 1		14866	3.8388	-	7470A	PPB	14 Apr 2021 13:32:34	U	SMPL
M2014-04DUPDLX50 - 1		15028	3.8818	-	7470A	PPB	14 Apr 2021 13:37:31	U	SMPL
M2014-04MSDL2X50 - 1		15845	4.0985	-	7470A	PPB	14 Apr 2021 13:39:46	U	SMPL
M2014-04MSDDL2X50 - 1		16771	4.3441	-	7470A	PPB	14 Apr 2021 13:42:02	U	SMPL
M2014-04LDL2X250 - 1		3048	0.7041	-	7470A	PPB	14 Apr 2021 13:44:17	U	SMPL
M2014-04ADL2X50 - 1		15698	4.0595	-	7470A	PPB	14 Apr 2021 13:46:33	U	SMPL
CCV05 - 1	CCV05	19893	5.1722	-	7470A	PPB	14 Apr 2021 13:51:25	U	SMPL
CCB05 - 1	CCB05	155	-0.0633	-	7470A	PPB	14 Apr 2021 13:53:41	U	SMPL