

LB114075

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

4/20/2021 16:37

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.988	0.0	0.104	
ICB1	-0.002	0.0	0.004	
CCV1	0.990	0.0	0.105	
CCB1	0.001	0.0	0.004	
PB135844BL	0.001	0.0	0.004	
PB135844BS	0.993	0.0	0.105	
M2078-01	0.010	0.0	0.005	
M2078-01DUP	0.011	0.0	0.005	
M2078-01MS	0.973	0.0	0.103	
M2078-01MSD	0.970	0.0	0.103	
CCV2	1.005	0.0	0.106	
CCB2	0.007	0.0	0.005	

N	12
Mean	0.496
SD	0.5129
CV%	103.49

Aquakem v. 7.2AQ1

Results from time period:

Tue Apr 20 16:20:17 2021

Tue Apr 20 16:35:16 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Phenolics-	P	0.0077	mg/l	4/20/2021 14:52:04	
0.05PPM	A	Phenolics-	P	0.0565	mg/l	4/20/2021 14:52:05	
0.1PPM	A	Phenolics-	P	0.107	mg/l	4/20/2021 14:52:06	
0.25PPM	A	Phenolics-	P	0.2533	mg/l	4/20/2021 14:52:07	
0.50PPM	A	Phenolics-	P	0.4914	mg/l	4/20/2021 14:52:08	
1.0PPM	A	Phenolics-	P	0.9659	mg/l	4/20/2021 14:52:09	
2.0PPM	A	Phenolics-	P	2.0183	mg/l	4/20/2021 14:52:10	
ICV1	S	Phenolics-	P	0.9884	mg/l	4/20/2021 16:20:18	
ICB1	S	Phenolics-	P	-0.002	mg/l	4/20/2021 16:20:19	
CCV1	S	Phenolics-	P	0.9901	mg/l	4/20/2021 16:20:22	
CCB1	S	Phenolics-	P	0.001	mg/l	4/20/2021 16:20:24	
PB135844BL	S	Phenolics-	P	0.0008	mg/l	4/20/2021 16:20:25	
PB135844BS	S	Phenolics-	P	0.9931	mg/l	4/20/2021 16:20:28	
M2078-01	S	Phenolics-	P	0.0098	mg/l	4/20/2021 16:30:19	
M2078-01DUP	S	Phenolics-	P	0.0114	mg/l	4/20/2021 16:30:22	
M2078-01MS	S	Phenolics-	P	0.9731	mg/l	4/20/2021 16:30:24	
M2078-01MSD	S	Phenolics-	P	0.9702	mg/l	4/20/2021 16:30:25	
CCV2	S	Phenolics-	P	1.0048	mg/l	4/20/2021 16:35:14	
CCB2	S	Phenolics-	P	0.0067	mg/l	4/20/2021 16:35:15	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : Am Instrument ID : Konelab

4/20/2021 14:57


Test Phenolics-

Accepted 4/20/2021 14:57

Factor 9.846
Bias 0.004

Coeff. of det. 0.999450

Errors

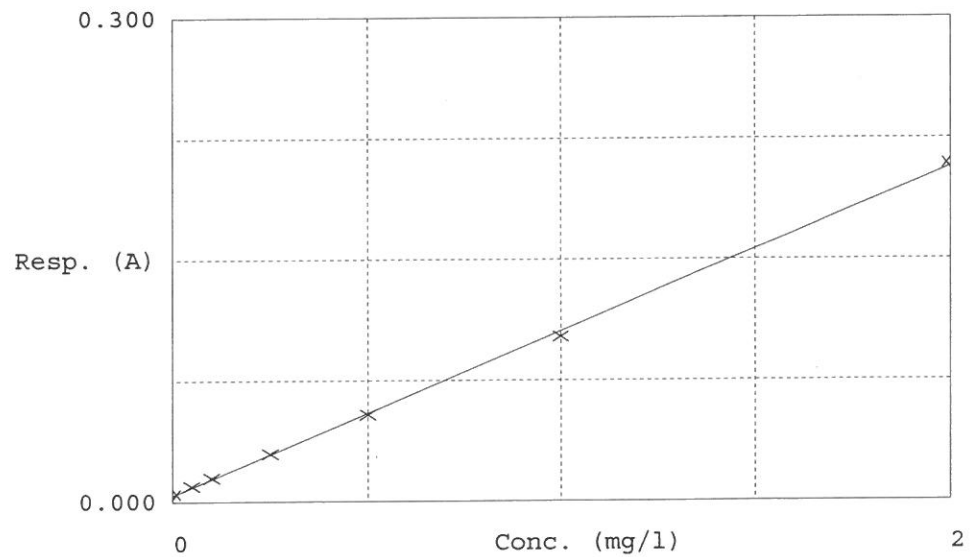

	Calibrator	Response	Calc. con.	Conc.	Errors %RE
1	0.00PPM	0.005	0.0077	0.0000	
2	Phenol-2	0.010	0.0565	0.0500	13.0
3	Phenol-2	0.015	0.1070	0.1000	7.0
4	Phenol-2	0.030	0.2533	0.2500	1.3
5	Phenol-2	0.054	0.4914	0.5000	-1.7
6	Phenol-2	0.102	0.9659	1.0000	-3.4
7	Phenol-2	0.209	2.0183	2.0000	0.9

04/20/2021
AM