


LB114082

7470A

INSTRUMENT ID: CV2

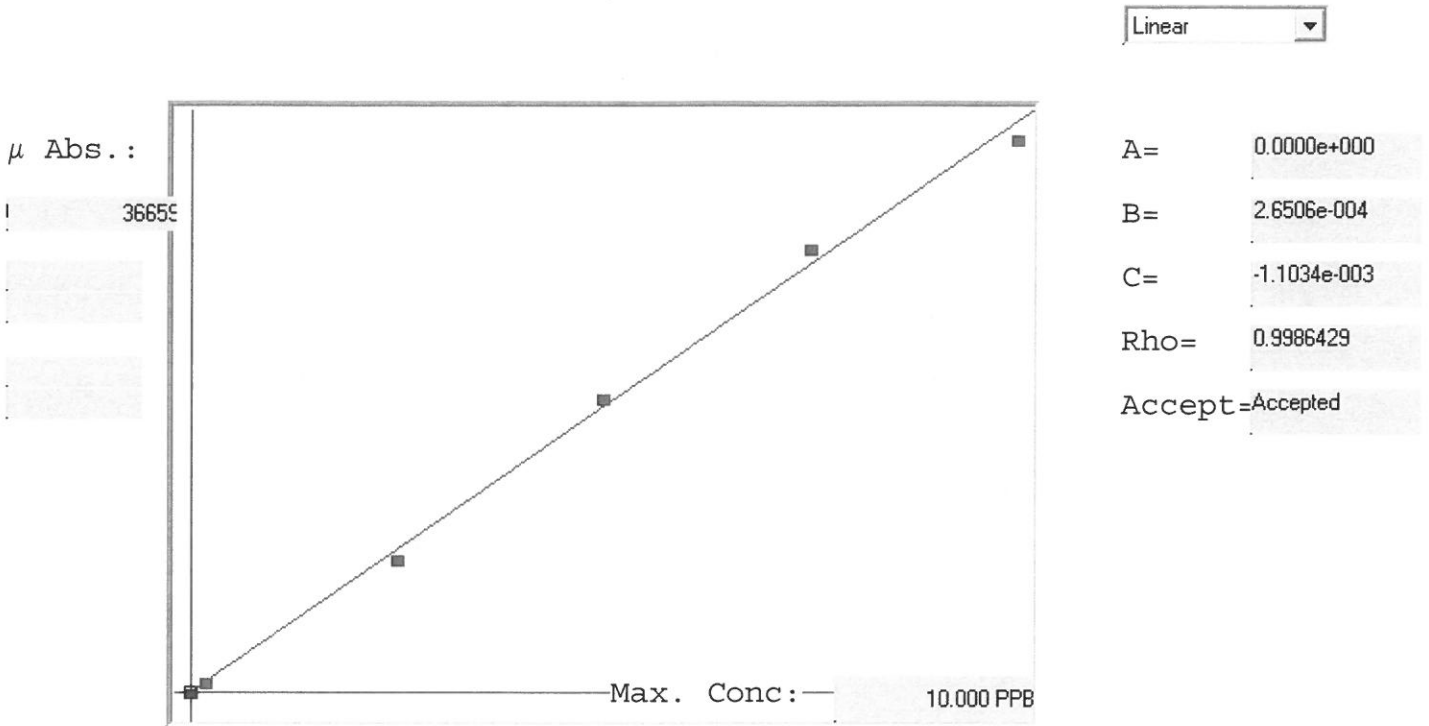

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/01
0.0	0.000	-0.003	-0.003	-7	0.000	-7					-4
0.2	0.200	0.192	-0.008	730	0.0 %	730					-7
2.5	2.500	2.336	-0.164	8816	0.0 %	8816					3
5.0	5.000	5.164	0.164	19487	0.0 %	19487					4
7.5	7.500	7.795	0.295	29411	0.0 %	29411					-3
10.0	10.000	9.716	-0.284	36659	0.0 %	36659					

LB114082 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 21 Apr 2021 11:03:54

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-7	-	0.0000	7470A	PPB	21 Apr 2021 11:08:17	S	Std
0.2 - 1	50.2	730	-	0.2000	7470A	PPB	21 Apr 2021 11:10:34	S	Std
2.5 - 1	52.5	8816	-	2.5000	7470A	PPB	21 Apr 2021 11:12:51	S	Std
5.0 - 1	55	19487	-	5.0000	7470A	PPB	21 Apr 2021 11:15:08	S	Std
7.5 - 1	57.5	29411	-	7.5000	7470A	PPB	21 Apr 2021 11:17:24	S	Std
10.0 - 1	510	36659	-	10.0000	7470A	PPB	21 Apr 2021 11:22:16	S	Std
ICV96 - 1	ICV96	14617	3.8734	-	7470A	PPB	21 Apr 2021 11:25:03	U	SMPL
ICB96 - 1	ICB96	-260	-0.0700	-	7470A	PPB	21 Apr 2021 11:27:17	U	SMPL
CCV57 - 1	CCV57	19720	5.2260	-	7470A	PPB	21 Apr 2021 11:29:32	U	SMPL
CCB57 - 1	CCB57	-257	-0.0692	-	7470A	PPB	21 Apr 2021 11:31:47	U	SMPL
CRA - 1	CRA	686	0.1807	-	7470A	PPB	21 Apr 2021 11:34:01	U	SMPL
HighStd - 1	HighStd	36872	9.7724	-	7470A	PPB	21 Apr 2021 11:36:16	U	SMPL
ChkStd - 1	ChkStd	27541	7.2991	-	7470A	PPB	21 Apr 2021 11:38:31	U	SMPL
PB135880BL - 1	PBW	-303	-0.0814	-	7470A	PPB	21 Apr 2021 11:40:48	U	SMPL
PB135880BS - 1	LCSW	14157	3.7514	-	7470A	PPB	21 Apr 2021 11:43:05	U	SMPL
M2090-04 - 1	SEDGWICK-COMP-1	-172	-0.0467	-	7470A	PPB	21 Apr 2021 11:45:21	U	SMPL
M2090-04DUP - 1	SEDGWICK-COMP-1DUP	4	-0.0000	-	7470A	PPB	21 Apr 2021 11:47:37	U	SMPL
M2090-04MS - 1	SEDGWICK-COMP-1MS	14918	3.9531	-	7470A	PPB	21 Apr 2021 11:49:54	U	SMPL
M2090-04MSD - 1	SEDGWICK-COMP-1MSD	16448	4.3587	-	7470A	PPB	21 Apr 2021 11:52:11	U	SMPL
M2090-09 - 1	SEDGWICK-COMP-2	-205	-0.0554	-	7470A	PPB	21 Apr 2021 11:54:26	U	SMPL
CCV58 - 1	CCV58	19779	5.2416	-	7470A	PPB	21 Apr 2021 11:56:42	U	SMPL
CCB58 - 1	CCB58	-228	-0.0615	-	7470A	PPB	21 Apr 2021 11:58:57	U	SMPL
M2090-14 - 1	SEDGWICK-COMP-3	-41	-0.0120	-	7470A	PPB	21 Apr 2021 12:01:12	U	SMPL
M2090-19 - 1	SEDGWICK-COMP-4	-4	-0.0022	-	7470A	PPB	21 Apr 2021 12:03:27	U	SMPL
M2090-23 - 1	SEDGWICK-COMP-5	18	0.0037	-	7470A	PPB	21 Apr 2021 12:05:42	U	SMPL
M2095-02 - 1	WC-1	17	0.0034	-	7470A	PPB	21 Apr 2021 12:07:58	U	SMPL
PB135881BL - 1	PBW	14	0.0026	-	7470A	PPB	21 Apr 2021 12:10:13	U	SMPL
PB135881BS - 1	LCSW	14352	3.8031	-	7470A	PPB	21 Apr 2021 12:12:29	U	SMPL
M1928-02 - 1	TW-4	4768	1.2627	-	7470A	PPB	21 Apr 2021 12:14:45	U	SMPL
M2078-02 - 1	TWP-01	794	0.2094	-	7470A	PPB	21 Apr 2021 12:21:54	U	SMPL
M2078-02DUP - 1	TWP-01DUP	684	0.1802	-	7470A	PPB	21 Apr 2021 12:24:11	U	SMPL
M2078-02MS - 1	TWP-01MS	17273	4.5774	-	7470A	PPB	21 Apr 2021 12:26:27	U	SMPL
CCV59 - 1	CCV59	19903	5.2745	-	7470A	PPB	21 Apr 2021 12:28:42	U	SMPL
CCB59 - 1	CCB59	-65	-0.0183	-	7470A	PPB	21 Apr 2021 12:30:57	U	SMPL
M2078-02MSD - 1	TWP-01MSD	16440	4.3566	-	7470A	PPB	21 Apr 2021 12:33:13	U	SMPL
M2078-03 - 1	TWP-01	107	0.0273	-	7470A	PPB	21 Apr 2021 12:35:28	U	SMPL
M2078-04 - 1	TWP-01-DULPlicate	271	0.0707	-	7470A	PPB	21 Apr 2021 12:37:44	U	SMPL
PB135880TB - 1	PB135855TB	53	0.0129	-	7470A	PPB	21 Apr 2021 12:39:59	U	SMPL
M2090-04LX5 - 1		31	0.0071	-	7470A	PPB	21 Apr 2021 12:42:15	U	SMPL
M2090-04A - 1		14774	3.9150	-	7470A	PPB	21 Apr 2021 12:44:31	U	SMPL
M2078-02LX5 - 1		264	0.0689	-	7470A	PPB	21 Apr 2021 12:46:47	U	SMPL
M2078-02A - 1		16767	4.4432	-	7470A	PPB	21 Apr 2021 12:49:04	U	SMPL
CCV60 - 1	CCV60	20074	5.3198	-	7470A	PPB	21 Apr 2021 12:51:21	U	SMPL
CCB60 - 1	CCB60	-72	-0.0202	-	7470A	PPB	21 Apr 2021 12:53:37	U	SMPL