


LB114196

7471B

INSTRUMENT ID: CV1

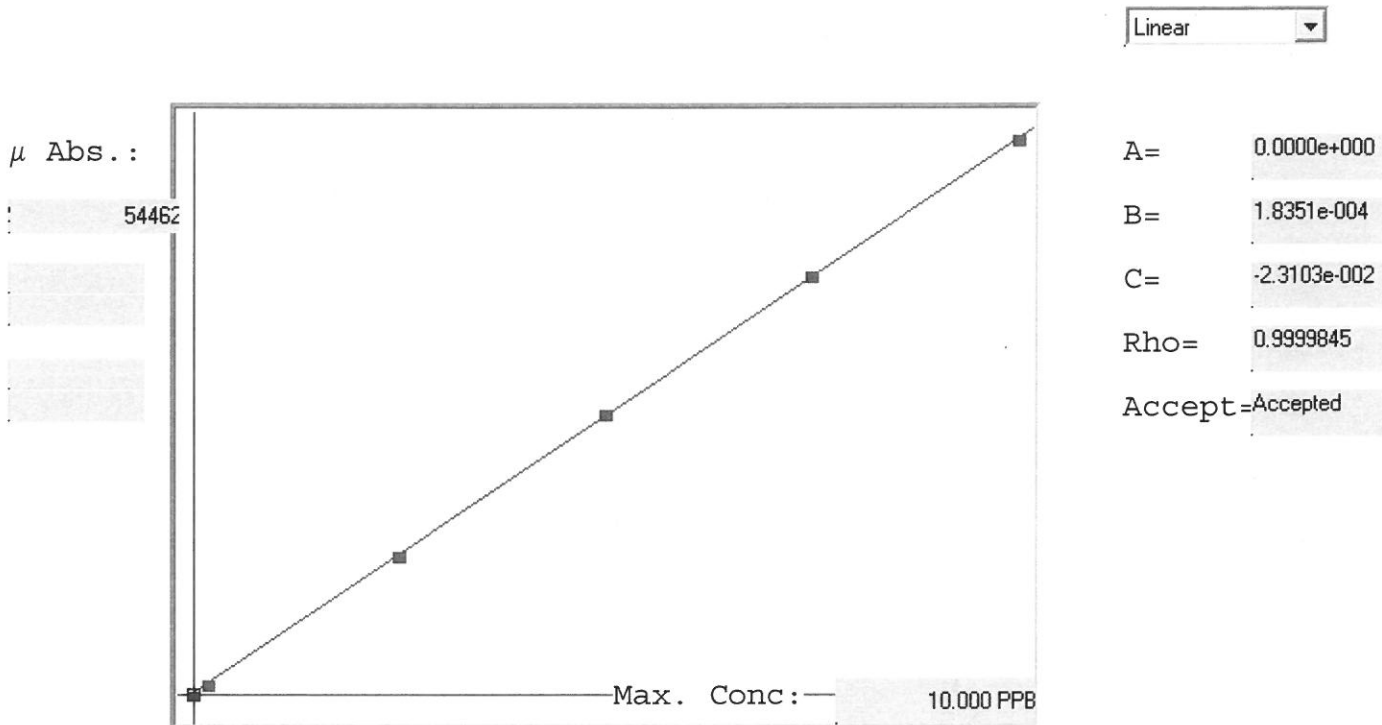

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.001	0.001	133	0.000	133					
0.2	0.200	0.181	-0.019	1114	0.0 %	1114					
2.5	2.500	2.496	-0.004	13725	0.0 %	13725					
5.0	5.000	5.032	0.032	27545	0.0 %	27545					
7.5	7.500	7.518	0.018	41095	0.0 %	41095					
10.0	10.000	9.971	-0.029	54462	0.0 %	54462					

0/01
-10
0
0
0
0

LB114196 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 28 Apr 2021 15:21:35

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	133	-	0.00007471B	PPB		28 Apr 2021 15:32:24	S	Std
0.2 - 1	50.2	1114	-	0.20007471B	PPB		28 Apr 2021 15:37:21	S	Std
2.5 - 1	52.5	13725	-	2.50007471B	PPB		28 Apr 2021 15:39:38	S	Std
5.0 - 1	55	27545	-	5.00007471B	PPB		28 Apr 2021 15:41:55	S	Std
7.5 - 1	57.5	41095	-	7.50007471B	PPB		28 Apr 2021 15:44:12	S	Std
10.0 - 1	510	54462	-	10.00007471B	PPB		28 Apr 2021 15:46:29	S	Std
ICV08 - 1	ICV08	22796	4.1603	-7471B	PPB		28 Apr 2021 15:52:01	U	SMPL
ICB08 - 1	ICB08	54	-0.0132	-7471B	PPB		28 Apr 2021 15:54:16	U	SMPL
CCV13 - 1	CCV13	28124	5.1381	-7471B	PPB		28 Apr 2021 15:56:32	U	SMPL
CCB13 - 1	CCB13	23	-0.0189	-7471B	PPB		28 Apr 2021 15:58:47	U	SMPL
CRA - 1	CRA	1117	0.1819	-7471B	PPB		28 Apr 2021 16:01:03	U	SMPL
HighStd - 1	HighStd	55362	10.1366	-7471B	PPB		28 Apr 2021 16:03:18	U	SMPL
ChkStd - 1	ChkStd	38119	6.9723	-7471B	PPB		28 Apr 2021 16:05:33	U	SMPL
PB136052BL - 1	PBS	-14	-0.0257	-7471B	PPB		28 Apr 2021 16:07:51	U	SMPL
PB136052BS - 1	LCSS	21956	4.0061	-7471B	PPB		28 Apr 2021 16:10:09	U	SMPL
M2188-01 - 1	TP-9A-8-COMP	5473	0.9813	-7471B	PPB		28 Apr 2021 16:12:26	U	SMPL
M2190-01 - 1	NB-08-042721	2830	0.4962	-7471B	PPB		28 Apr 2021 16:14:43	U	SMPL
M2191-01 - 1	TR-05-042721	2433	0.4234	-7471B	PPB		28 Apr 2021 16:17:00	U	SMPL
M2193-01 - 1	S-1	1351	0.2248	-7471B	PPB		28 Apr 2021 16:19:17	U	SMPL
M2196-01 - 1	WALL-D-4075-A	3239	0.5713	-7471B	PPB		28 Apr 2021 16:21:32	U	SMPL
CCV14 - 1	CCV14	28262	5.1634	-7471B	PPB		28 Apr 2021 16:23:47	U	SMPL
CCB14 - 1	CCB14	-72	-0.0363	-7471B	PPB		28 Apr 2021 16:26:03	U	SMPL
M2196-05 - 1	WALL-D-4075-B	3649	0.6465	-7471B	PPB		28 Apr 2021 16:28:18	U	SMPL
M2198-01 - 1	SAMPLE-1-GRAB	10293	1.8658	-7471B	PPB		28 Apr 2021 16:30:33	U	SMPL
M2199-03 - 1	SAMPLE-3-COMP	10429	1.8908	-7471B	PPB		28 Apr 2021 16:37:43	U	SMPL
M2199-03DUP - 1	SAMPLE-3-COMPDUP	11613	2.1081	-7471B	PPB		28 Apr 2021 16:39:58	U	SMPL
M2199-03MS - 1	SAMPLE-3-COMPMS	31551	5.7670	-7471B	PPB		28 Apr 2021 16:42:14	U	SMPL
M2199-03MSD - 1	SAMPLE-3-COMPMSD	34293	6.2702	-7471B	PPB		28 Apr 2021 16:47:21	U	SMPL
M2199-03LX5 - 1		1761	0.3001	-7471B	PPB		28 Apr 2021 16:49:38	U	SMPL
M2199-03A - 1		32738	5.9848	-7471B	PPB		28 Apr 2021 16:51:56	U	SMPL
CCV15 - 1	CCV15	28615	5.2282	-7471B	PPB		28 Apr 2021 16:54:13	U	SMPL
CCB15 - 1	CCB15	-73	-0.0365	-7471B	PPB		28 Apr 2021 16:56:29	U	SMPL