


LB114267

7470A

INSTRUMENT ID: CV1

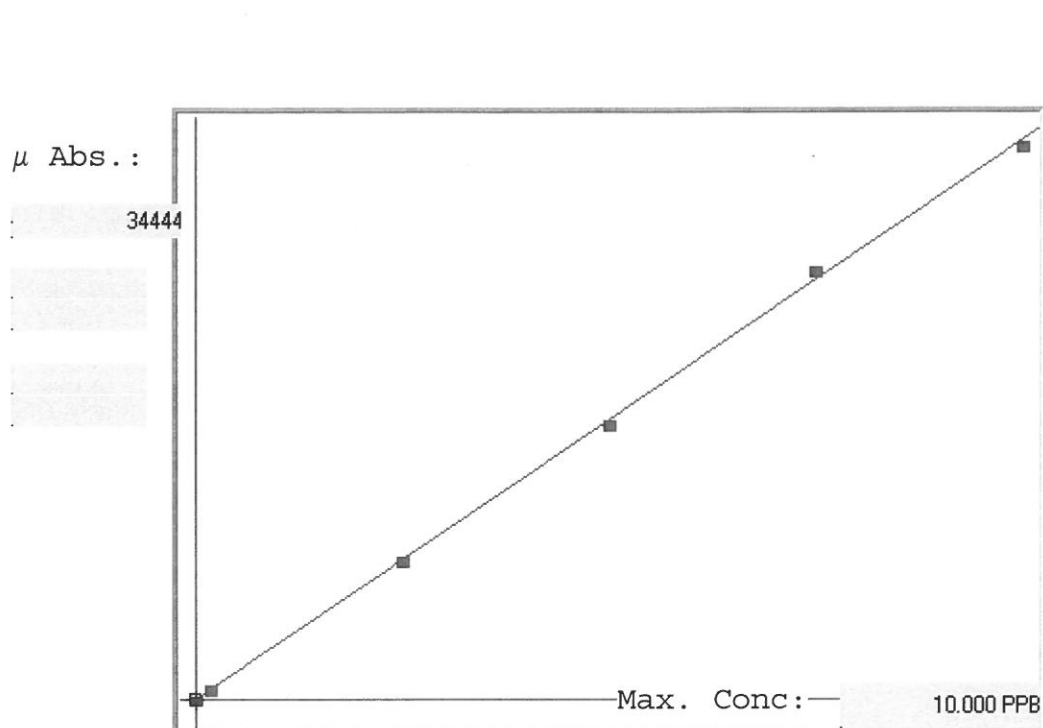

Linear

A= 0.0000e+000

B= 2.8768e-004

C= 6.9647e-003

Rho= 0.9997831

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	90h
0.0	0.000	0.006	0.006	-5	0.000	-5					3
0.2	0.200	0.206	0.006	693	0.0 %	693					1
2.5	2.500	2.478	-0.022	8589	0.0 %	8589					1
5.0	5.000	4.939	-0.061	17145	0.0 %	17145					2
7.5	7.500	7.655	0.155	26586	0.0 %	26586					1
10.0	10.000	9.916	-0.084	34444	0.0 %	34444					

LB114267 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 May 2021 10:55:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-5	-	0.0000	7470A	PPB	04 May 2021 10:57:46	S	Std
0.2 - 1	50.2	693	-	0.2000	7470A	PPB	04 May 2021 11:00:03	S	Std
2.5 - 1	52.5	8589	-	2.5000	7470A	PPB	04 May 2021 11:02:20	S	Std
5.0 - 1	55	17145	-	5.0000	7470A	PPB	04 May 2021 11:04:37	S	Std
7.5 - 1	57.5	26586	-	7.5000	7470A	PPB	04 May 2021 11:09:26	S	Std
10.0 - 1	510	34444	-	10.0000	7470A	PPB	04 May 2021 11:14:20	S	Std
ICV15 - 1	ICV15	13897	4.0049	-7470A	PPB	PPB	04 May 2021 11:17:01	U	SMPL
ICB15 - 1	ICB15	-210	-0.0534	-7470A	PPB	PPB	04 May 2021 11:19:16	U	SMPL
CCV37 - 1	CCV37	17512	5.0448	-7470A	PPB	PPB	04 May 2021 11:21:32	U	SMPL
CCB37 - 1	CCB37	-198	-0.0500	-7470A	PPB	PPB	04 May 2021 11:23:47	U	SMPL
CRA - 1	CRA	642	0.1917	-7470A	PPB	PPB	04 May 2021 11:26:02	U	SMPL
HighStd - 1	HighStd	34002	9.7887	-7470A	PPB	PPB	04 May 2021 11:28:17	U	SMPL
ChkStd - 1	ChkStd	24370	7.0177	-7470A	PPB	PPB	04 May 2021 11:30:32	U	SMPL
PB136148BL - 1	PBW	-251	-0.0652	-7470A	PPB	PPB	04 May 2021 11:32:50	U	SMPL
PB136148BS - 1	LCSW	12576	3.6248	-7470A	PPB	PPB	04 May 2021 11:35:07	U	SMPL
M2246-01 - 1	FILL-A	131	0.0447	-7470A	PPB	PPB	04 May 2021 11:37:23	U	SMPL
M2246-01DUP - 1	FILL-ADUP	-13	0.0032	-7470A	PPB	PPB	04 May 2021 11:42:21	U	SMPL
M2246-01MS - 1	FILL-AMS	12345	3.5584	-7470A	PPB	PPB	04 May 2021 11:47:10	U	SMPL
M2246-01MSD - 1	FILL-AMSD	12497	3.6021	-7470A	PPB	PPB	04 May 2021 11:49:27	U	SMPL
M2246-02 - 1	FILL-B	-92	-0.0195	-7470A	PPB	PPB	04 May 2021 11:51:42	U	SMPL
CCV38 - 1	CCV38	16699	4.8109	-7470A	PPB	PPB	04 May 2021 11:53:58	U	SMPL
CCB38 - 1	CCB38	-158	-0.0385	-7470A	PPB	PPB	04 May 2021 11:56:14	U	SMPL
M2246-03 - 1	FILL-C	24	0.0139	-7470A	PPB	PPB	04 May 2021 11:58:31	U	SMPL
PB136148TB - 1	PB136108TB	0	0.0070	-7470A	PPB	PPB	04 May 2021 12:00:47	U	SMPL
M2246-01LX5 - 1		24	0.0139	-7470A	PPB	PPB	04 May 2021 12:03:02	U	SMPL
M2246-01A - 1		13346	3.8463	-7470A	PPB	PPB	04 May 2021 12:05:18	U	SMPL
CCV39 - 1	CCV39	17033	4.9070	-7470A	PPB	PPB	04 May 2021 12:07:33	U	SMPL
CCB39 - 1	CCB39	-192	-0.0483	-7470A	PPB	PPB	04 May 2021 12:09:49	U	SMPL