

LB114381

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : Am Instrument ID : Konelab

5/11/2021 14:17

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.967	0.0	0.108	
ICB1	-0.003	0.0	0.004	
CCV1	0.964	0.0	0.107	
CCB1	-0.003	0.0	0.004	
PB136272BL	-0.004	0.0	0.004	
PB136272BS	0.964	0.0	0.107	
M2262-10	0.024	0.0	0.007	
M2262-11	0.047	0.0	0.010	
M2307-03	0.098	0.0	0.015	
M2307-03DUP	0.097	0.0	0.015	
M2307-03MS	0.952	0.0	0.106	
M2307-03MSD	0.956	0.0	0.107	
M2307-04	0.001	0.0	0.005	
CCV2	0.965	0.0	0.108	
CCB2	-0.004	0.0	0.004	

N	15
Mean	0.401
SD	0.4745
CV%	118.18

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

5/11/2021 13:32


Test Phenolics-

Accepted 5/11/2021 13:32

Factor 9.375
Bias 0.005

Coeff. of det. 0.999988

Errors

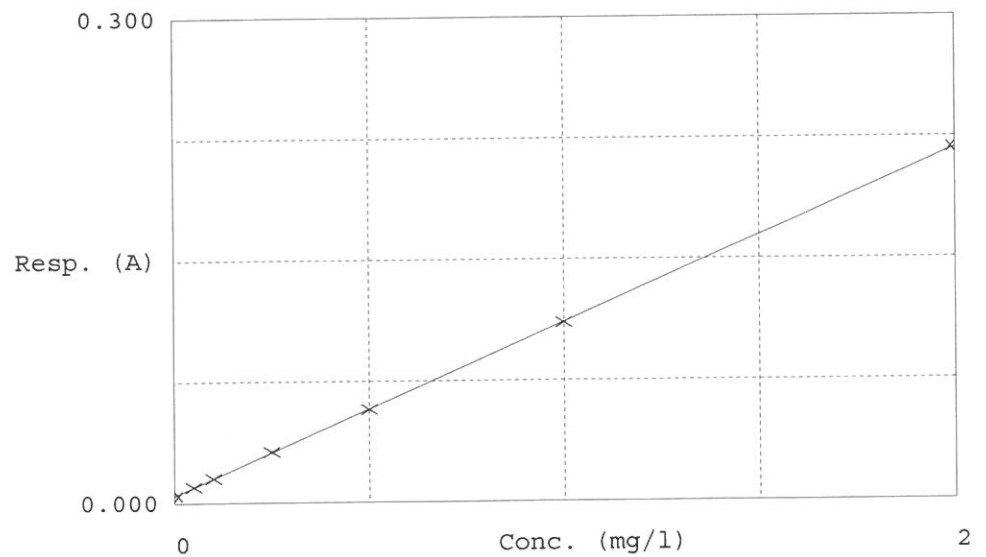

	Calibrator	Response	Calc. con.	Conc.	Errors %RE
1	0.00PPM	0.005	-0.0004	0.0000	
2	Phenol-2	0.010	0.0509	0.0500	1.8
3	Phenol-2	0.015	0.1004	0.1000	0.4
4	Phenol-2	0.032	0.2532	0.2500	1.3
5	Phenol-2	0.058	0.4978	0.5000	-0.4
6	Phenol-2	0.111	0.9960	1.0000	-0.4
7	Phenol-2	0.218	2.0021	2.0000	0.1

05/11/2021
AM

Aquakem v. 7.2AQ1

Results from time period:

Tue May 11 13:30:16 2021

Tue May 11 14:08:43 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Phenolics-	P	-0.0004	mg/l	5/11/2021 13:30:16	
0.05PPM	A	Phenolics-	P	0.0509	mg/l	5/11/2021 13:30:17	
0.1PPM	A	Phenolics-	P	0.1004	mg/l	5/11/2021 13:30:18	
0.25PPM	A	Phenolics-	P	0.2532	mg/l	5/11/2021 13:30:19	
0.50PPM	A	Phenolics-	P	0.4978	mg/l	5/11/2021 13:30:20	
1.0PPM	A	Phenolics-	P	0.996	mg/l	5/11/2021 13:30:21	
2.0PPM	A	Phenolics-	P	2.0021	mg/l	5/11/2021 13:30:22	
ICV1	S	Phenolics-	P	0.967	mg/l	5/11/2021 13:58:39	
ICB1	S	Phenolics-	P	-0.0032	mg/l	5/11/2021 13:58:40	
CCV1	S	Phenolics-	P	0.9642	mg/l	5/11/2021 13:58:43	
CCB1	S	Phenolics-	P	-0.0026	mg/l	5/11/2021 13:58:44	
PB136272BL	S	Phenolics-	P	-0.0038	mg/l	5/11/2021 13:58:46	
PB136272BS	S	Phenolics-	P	0.9644	mg/l	5/11/2021 13:58:47	
M2262-10	S	Phenolics-	P	0.0236	mg/l	5/11/2021 13:58:49	
M2262-11	S	Phenolics-	P	0.0475	mg/l	5/11/2021 14:08:33	
M2307-03	S	Phenolics-	P	0.0976	mg/l	5/11/2021 14:08:35	
M2307-03DUP	S	Phenolics-	P	0.0975	mg/l	5/11/2021 14:08:36	
M2307-03MS	S	Phenolics-	P	0.9522	mg/l	5/11/2021 14:08:37	
M2307-03MSD	S	Phenolics-	P	0.9562	mg/l	5/11/2021 14:08:38	
M2307-04	S	Phenolics-	P	0.0006	mg/l	5/11/2021 14:08:39	
CCV2	S	Phenolics-	P	0.9651	mg/l	5/11/2021 14:08:40	
CCB2	S	Phenolics-	P	-0.0043	mg/l	5/11/2021 14:08:42	