


LB114396

7471B

INSTRUMENT ID: CV2

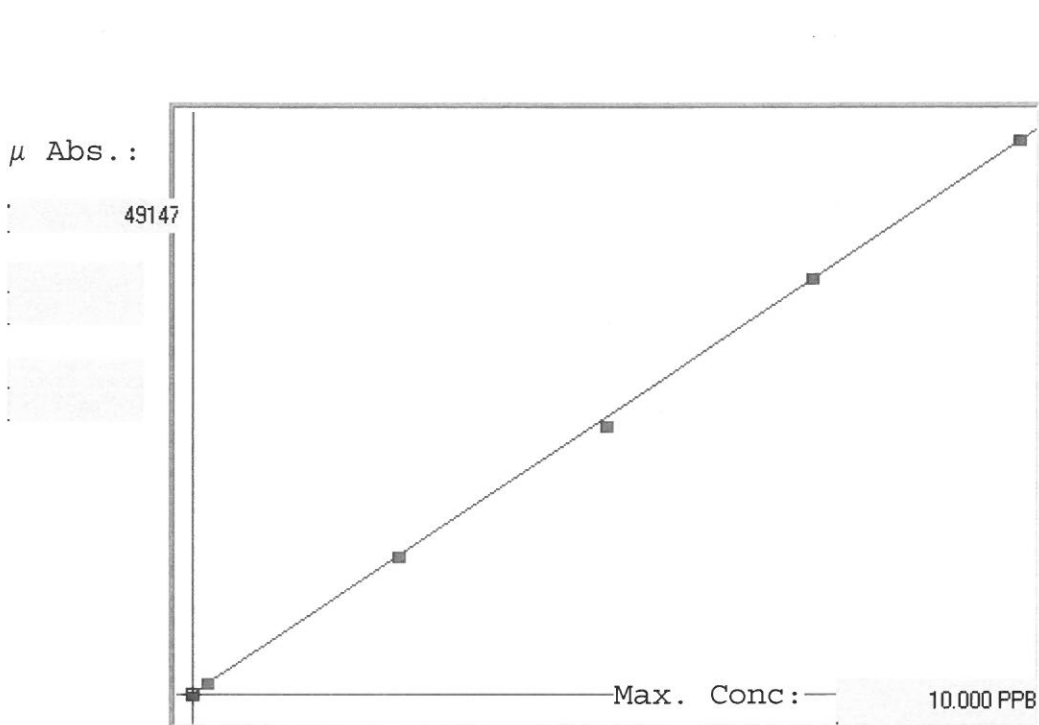

Linear

A= 0.0000e+000

B= 2.0410e-004

C= -3.2296e-003

Rho= 0.9999054

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.012	0.012	73	0.000	73					6/01
0.2	0.200	0.226	0.026	1125	0.0 %	1125					13
2.5	2.500	2.517	0.017	12349	0.0 %	12349					1
5.0	5.000	4.887	-0.113	23962	0.0 %	23962					2
7.5	7.500	7.530	0.030	36909	0.0 %	36909					0
10.0	10.000	10.028	0.028	49147	0.0 %	49147					0

LB114396 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 12 May 2021 08:43:08					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	73	-	0.0000	7471B	PPB	12 May 2021 08:51:54	S	Std
0.2 - 1	Si.2	1125	-	0.2000	7471B	PPB	12 May 2021 08:54:11	S	Std
2.5 - 1	Si.5	12349	-	2.5000	7471B	PPB	12 May 2021 08:56:28	S	Std
5.0 - 1	Si.5	23962	-	5.0000	7471B	PPB	12 May 2021 08:58:44	S	Std
7.5 - 1	Si.5	36909	-	7.5000	7471B	PPB	12 May 2021 09:01:01	S	Std
10.0 - 1	Si.0	49147	-	10.0000	7471B	PPB	12 May 2021 09:03:18	S	Std
ICV22 - 1	ICV22	19222	3.9199		7471B	PPB	12 May 2021 09:06:02	U	SMPL
ICB22 - 1	ICB22	-155	-0.0349		7471B	PPB	12 May 2021 09:08:16	U	SMPL
CCV61 - 1	CCV61	24582	5.0139		7471B	PPB	12 May 2021 09:13:11	U	SMPL
CCB61 - 1	CCB61	-167	-0.0373		7471B	PPB	12 May 2021 09:15:26	U	SMPL
CRA - 1	CRA	1072	0.2156		7471B	PPB	12 May 2021 09:17:44	U	SMPL
HighStd - 1	HighStd	49273	10.0533		7471B	PPB	12 May 2021 09:19:59	U	SMPL
ChkStd - 1	ChkStd	34238	6.9847		7471B	PPB	12 May 2021 09:22:14	U	SMPL
PB136321BL - 1	PBS	-21	-0.0075		7471B	PPB	12 May 2021 09:27:06	U	SMPL
PB136321BS - 1	LCSS	19194	3.9142		7471B	PPB	12 May 2021 09:32:03	U	SMPL
M2277-01 - 1	FK-BPM-01-A3-A3A-B3-B3A	836	0.1674		7471B	PPB	12 May 2021 09:34:19	U	SMPL
M2295-01 - 1	DRUM-A-B-C	504	0.0996		7471B	PPB	12 May 2021 09:36:37	U	SMPL
M2295-05 - 1	DRUM-D-E	1274	0.2568		7471B	PPB	12 May 2021 09:38:53	U	SMPL
M2296-01 - 1	SP-1	1296	0.2613		7471B	PPB	12 May 2021 09:41:11	U	SMPL
M2305-01 - 1	P-1	3021	0.6134		7471B	PPB	12 May 2021 09:43:25	U	SMPL
CCV62 - 1	CCV62	24143	4.9243		7471B	PPB	12 May 2021 09:45:40	U	SMPL
CCB62 - 1	CCB62	-69	-0.0173		7471B	PPB	12 May 2021 09:47:56	U	SMPL
M2306-01 - 1	C-1	2189	0.4435		7471B	PPB	12 May 2021 09:50:12	U	SMPL
M2330-01 - 1	CFOS-SOIL	1771	0.3582		7471B	PPB	12 May 2021 09:52:27	U	SMPL
M2330-01DUP - 1	CFOS-SOILDUP	1644	0.3323		7471B	PPB	12 May 2021 09:54:42	U	SMPL
M2330-01MS - 1	CFOS-SOILMS	20269	4.1336		7471B	PPB	12 May 2021 09:56:58	U	SMPL
M2330-01MSD - 1	CFOS-SOILMSD	20285	4.1369		7471B	PPB	12 May 2021 09:59:13	U	SMPL
M2335-01 - 1	OK-02-050721	3496	0.7103		7471B	PPB	12 May 2021 10:01:31	U	SMPL
M2330-01LX5 - 1		359	0.0700		7471B	PPB	12 May 2021 10:03:48	U	SMPL
M2330-01A - 1		21950	4.4767		7471B	PPB	12 May 2021 10:06:05	U	SMPL
CCV63 - 1	CCV63	24518	5.0008		7471B	PPB	12 May 2021 10:08:22	U	SMPL
CCB63 - 1	CCB63	-80	-0.0196		7471B	PPB	12 May 2021 10:10:39	U	SMPL