


LB 114401

245.1

INSTRUMENT ID: CV1

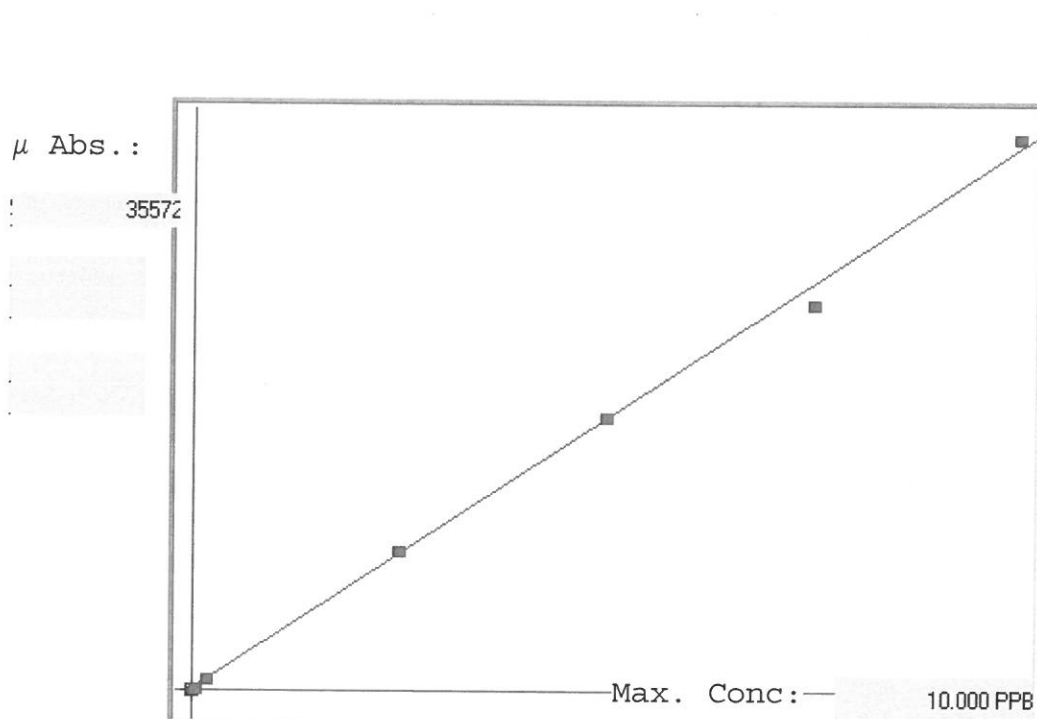

Linear

A= 0.0000e+000

B= 2.8716e-004

C= -1.6128e-002

Rho= 0.9990512

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.001	0.001	58	0.000	58					
0.05	0.050	0.055	0.005	246	0.0 %	246	0				10
0.2	0.200	0.212	0.012	794	0.0 %	794					6
2.5	2.500	2.574	0.074	9021	0.0 %	9021					3
5.0	5.000	5.074	0.074	17724	0.0 %	17724					1
7.5	7.500	7.136	-0.364	24907	0.0 %	24907					5
10.0	10.000	10.199	0.199	35572	0.0 %	35572					2

LB114401 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 12 May 2021 11:49:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	58	-	0.0000	245.1	PPB	12 May 2021 12:03:54	S	Std
0.05 - 1	50.05	246	-	0.0500	245.1	PPB	12 May 2021 12:06:11	S	Std
0.2 - 1	50.2	794	-	0.2000	245.1	PPB	12 May 2021 12:08:28	S	Std
2.5 - 1	52.5	9021	-	2.5000	245.1	PPB	12 May 2021 12:10:45	S	Std
5.0 - 1	55	17724	-	5.0000	245.1	PPB	12 May 2021 12:13:01	S	Std
7.5 - 1	57.5	24907	-	7.5000	245.1	PPB	12 May 2021 12:20:16	S	Std
10.0 - 1	510	35572	-	10.0000	245.1	PPB	12 May 2021 12:28:01	S	Std
ICV23 - 1	ICV23	14280	4.0846	-245.1		PPB	12 May 2021 12:30:52	U	SMPL
ICB23 - 1	ICB23	-88	-0.0414	-245.1		PPB	12 May 2021 12:33:06	U	SMPL
CCV64 - 1	CCV64	17874	5.1166	-245.1		PPB	12 May 2021 12:35:22	U	SMPL
CCB64 - 1	CCB64	-72	-0.0368	-245.1		PPB	12 May 2021 12:37:37	U	SMPL
CRA - 1	CRA	206	0.0430	-245.1		PPB	12 May 2021 12:39:54	U	SMPL
HighStd - 1	HighStd	35448	10.1633	-245.1		PPB	12 May 2021 12:42:09	U	SMPL
ChkStd - 1	ChkStd	23402	6.7041	-245.1		PPB	12 May 2021 12:44:24	U	SMPL
PB136343BL - 1	PBW	-101	-0.0451	-245.1		PPB	12 May 2021 12:46:42	U	SMPL
PB136343BS - 1	LCSW	15226	4.3562	-245.1		PPB	12 May 2021 12:49:03	U	SMPL
M2257-07 - 1	14B-(1-4)-COMP	826	0.2211	-245.1		PPB	12 May 2021 12:51:20	U	SMPL
M2274-07 - 1	14B-(1-4)-COMP	440	0.1102	-245.1		PPB	12 May 2021 12:56:43	U	SMPL
M2297-01 - 1	COMP	369	0.0898	-245.1		PPB	12 May 2021 12:58:59	U	SMPL
M2307-03 - 1	MW-05	264	0.0597	-245.1		PPB	12 May 2021 13:01:16	U	SMPL
CCV65 - 1	CCV65	16981	4.8602	-245.1		PPB	12 May 2021 13:03:31	U	SMPL
CCB65 - 1	CCB65	-36	-0.0265	-245.1		PPB	12 May 2021 13:05:47	U	SMPL
M2307-04 - 1	MW-18	1283	0.3523	-245.1		PPB	12 May 2021 13:13:07	U	SMPL
M2307-04DUP - 1	MW-18DUP	1221	0.3345	-245.1		PPB	12 May 2021 13:15:22	U	SMPL
M2307-04MS - 1	MW-18MS	15811	4.5242	-245.1		PPB	12 May 2021 13:17:37	U	SMPL
M2307-04MSD - 1	MW-18MSD	14259	4.0785	-245.1		PPB	12 May 2021 13:19:51	U	SMPL
M2352-07 - 1	14B-(1-4)-COMP	333	0.0795	-245.1		PPB	12 May 2021 13:22:07	U	SMPL
M2359-07 - 1	14B-(1-4)-COMP	532	0.1366	-245.1		PPB	12 May 2021 13:24:23	U	SMPL
M2307-04LX5 - 1		250	0.0557	-245.1		PPB	12 May 2021 13:26:39	U	SMPL
M2307-04A - 1		15045	4.3043	-245.1		PPB	12 May 2021 13:28:56	U	SMPL
CCV66 - 1	CCV66	16530	4.7307	-245.1		PPB	12 May 2021 13:31:13	U	SMPL
CCB66 - 1	CCB66	-50	-0.0305	-245.1		PPB	12 May 2021 13:33:29	U	SMPL