

LB114418


SFAM01.1

INSTRUMENT ID: CV1

Linear

μ Abs.:

41416

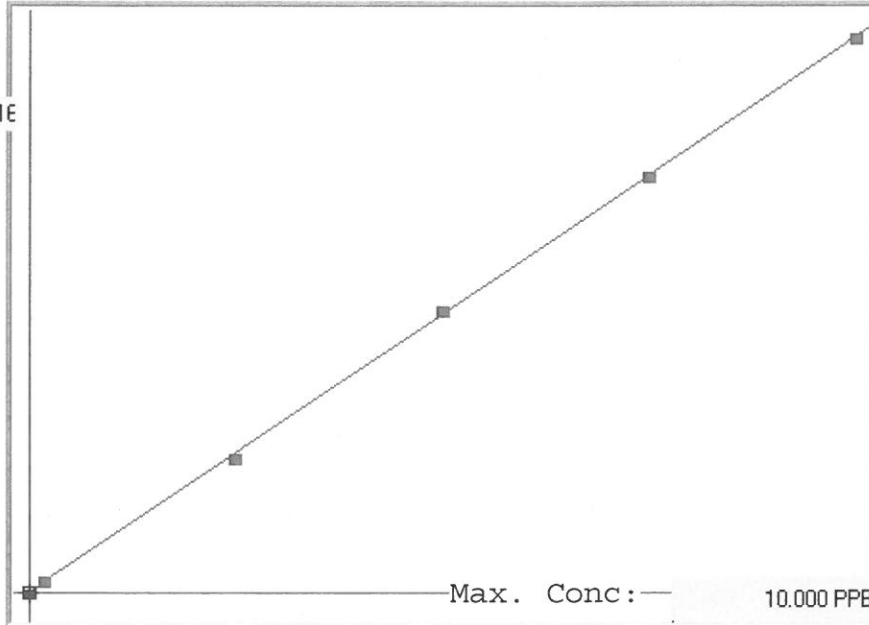

A= 0.0000e+000

B= 2.4114e-004 *slope*

C= -1.0809e-002 *y-intercept*

Rho= 0.9999228

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.009	0.009	82	0.000	82					11
0.05	0.050					204					2
0.20	0.200	0.204	0.004	891	0.0 %	891					3
2.50	2.500	2.430	-0.070	10120	0.0 %	10120					2
5.00	5.000	5.084	0.084	21126	0.0 %	21126					0
7.50	7.500	7.497	-0.003	31136	0.0 %	31136					0
10.0	10.000	9.976	-0.024	41416	0.0 %	41416					0

LB114418
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	82	-		0 SFAM01.1	PPB	5/12/2021 16:27	Std
	0.2 S01	891	-		0.2 SFAM01.1	PPB	5/12/2021 16:29	Std
	2.5 S02	10120	-		2.5 SFAM01.1	PPB	5/12/2021 16:32	Std
	5 S03	21126	-		5 SFAM01.1	PPB	5/12/2021 16:34	Std
	7.5 S04	31136	-		7.5 SFAM01.1	PPB	5/12/2021 16:36	Std
	10 S05	41416	-		10 SFAM01.1	PPB	5/12/2021 16:39	Std
ICV020	ICV020	15678	3.7698 -		SFAM01.1	PPB	5/12/2021 16:41	SMPL
ICB020	ICB020	-69	-0.0274 -		SFAM01.1	PPB	5/12/2021 16:44	SMPL
CCV070	CCV070	21101	5.0776 -		SFAM01.1	PPB	5/12/2021 16:46	SMPL
CCB070	CCB070	-86	-0.0315 -		SFAM01.1	PPB	5/12/2021 16:48	SMPL
PB136346BL	PBW346	62	0.0041 -		SFAM01.1	PPB	5/12/2021 16:53	SMPL
M2248-01	MHOAA0	324	0.0673 -		SFAM01.1	PPB	5/12/2021 16:55	SMPL
M2248-02	MHOAA1	322	0.0668 -		SFAM01.1	PPB	5/12/2021 16:57	SMPL
M2248-03	MHOAA2	288	0.0586 -		SFAM01.1	PPB	5/12/2021 17:00	SMPL
M2248-04	MHOAA3	326	0.0678 -		SFAM01.1	PPB	5/12/2021 17:02	SMPL
M2248-05	MHOAA4	252	0.05 -		SFAM01.1	PPB	5/12/2021 17:04	SMPL
M2248-06	MHOAA4D	227	0.0439 -		SFAM01.1	PPB	5/12/2021 17:06	SMPL
M2248-07	MHOAA4S	4333	1.0341 -		SFAM01.1	PPB	5/12/2021 17:13	SMPL
M2248-08	MHOAA5	63	0.0044 -		SFAM01.1	PPB	5/12/2021 17:15	SMPL
M2248-09	MHOAA6	86	0.0099 -		SFAM01.1	PPB	5/12/2021 17:17	SMPL
M2248-10	MHOAA7	197	0.0367 -		SFAM01.1	PPB	5/12/2021 17:20	SMPL
M2248-11	MHOAA8	187	0.0343 -		SFAM01.1	PPB	5/12/2021 17:22	SMPL
M2248-12	MHOAA9	135	0.0217 -		SFAM01.1	PPB	5/12/2021 17:24	SMPL
M2248-13	MHOAB0	160	0.0278 -		SFAM01.1	PPB	5/12/2021 17:26	SMPL
M2248-14	MHOAB1	120	0.0181 -		SFAM01.1	PPB	5/12/2021 17:29	SMPL
M2248-15	MHOAB2	375	0.0796 -		SFAM01.1	PPB	5/12/2021 17:31	SMPL
M2248-16	MHOAB3	218	0.0418 -		SFAM01.1	PPB	5/12/2021 17:33	SMPL
M2248-17	MHOAB4	227	0.0439 -		SFAM01.1	PPB	5/12/2021 17:35	SMPL
CCV071	CCV071	20823	5.0105 -		SFAM01.1	PPB	5/12/2021 17:38	SMPL
CCB071	CCB071	-76	-0.0291 -		SFAM01.1	PPB	5/12/2021 17:40	SMPL