

LB114441


7470A

INSTRUMENT ID: CV2

Linear

 μ Abs.:

38318

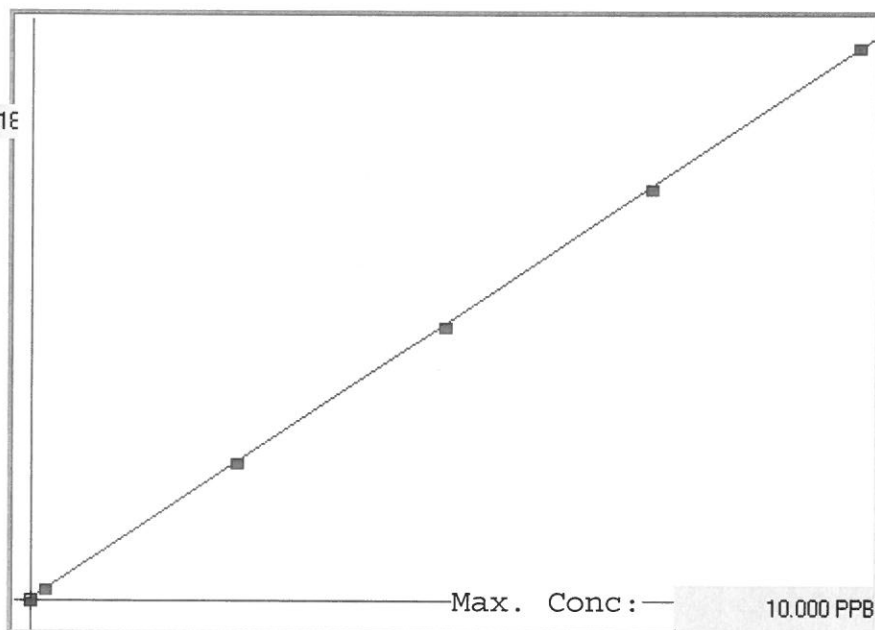

A= 0.0000e+000

B= 2.6200e-004

C= -1.3713e-002

Rho= 0.9999879

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.012	0.012	99	0.000	99					1
0.2	0.200	0.201	0.001	818	0.0 %	818					0
2.5	2.500	2.508	0.008	9624	0.0 %	9624					0
5.0	5.000	4.972	-0.028	19031	0.0 %	19031					-1
7.5	7.500	7.481	-0.019	28607	0.0 %	28607					0
10.0	10.000	10.026	0.026	38318	0.0 %	38318					6

LB114441 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 May 2021 14:29:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	99	-	0.0000	7470A	PPB	13 May 2021 14:30:07	S	Std
0.2 - 1	50.2	818	-	0.2000	7470A	PPB	13 May 2021 14:32:24	S	Std
2.5 - 1	52.5	9624	-	2.5000	7470A	PPB	13 May 2021 14:34:41	S	Std
5.0 - 1	55	19031	-	5.0000	7470A	PPB	13 May 2021 14:36:58	S	Std
7.5 - 1	57.5	28607	-	7.5000	7470A	PPB	13 May 2021 14:39:14	S	Std
10.0 - 1	510	38318	-	10.0000	7470A	PPB	13 May 2021 14:41:31	S	Std
ICV25 - 1	ICV25	14812	3.8670	-	7470A	PPB	13 May 2021 14:44:16	U	SMPL
ICB25 - 1	ICB25	-70	-0.0321	-	7470A	PPB	13 May 2021 14:46:31	U	SMPL
CCV74 - 1	CCV74	18687	4.8823	-	7470A	PPB	13 May 2021 14:50:37	U	SMPL
CCB74 - 1	CCB74	-80	-0.0347	-	7470A	PPB	13 May 2021 14:52:51	U	SMPL
CRA - 1	CRA	750	0.1828	-	7470A	PPB	13 May 2021 14:55:07	U	SMPL
HighStd - 1	HighStd	38288	10.0178	-	7470A	PPB	13 May 2021 14:57:21	U	SMPL
ChkStd - 1	ChkStd	26698	6.9812	-	7470A	PPB	13 May 2021 14:59:37	U	SMPL
PB136374BL - 1	PBW	-127	-0.0470	-	7470A	PPB	13 May 2021 15:01:54	U	SMPL
PB136374BS - 1	LCSW	15416	4.0253	-	7470A	PPB	13 May 2021 15:04:11	U	SMPL
M2362-01 - 1	149TH-ST-DRUM-1-PPE	-53	-0.0276	-	7470A	PPB	13 May 2021 15:06:27	U	SMPL
M2362-02 - 1	TREMONT-AVE-DRUM-8-PPE	103	0.0133	-	7470A	PPB	13 May 2021 15:08:44	U	SMPL
M2362-03 - 1	TREMONT-AVE-DRUM-9-POLY	37	-0.0040	-	7470A	PPB	13 May 2021 15:11:01	U	SMPL
M2364-02 - 1	AST2-COPR4-1	131	0.0206	-	7470A	PPB	13 May 2021 15:13:18	U	SMPL
M2364-02DUP - 1	AST2-COPR4-1DUP	47	-0.0014	-	7470A	PPB	13 May 2021 15:15:33	U	SMPL
CCV75 - 1	CCV75	18443	4.8184	-	7470A	PPB	13 May 2021 15:17:49	U	SMPL
CCB75 - 1	CCB75	-87	-0.0365	-	7470A	PPB	13 May 2021 15:20:04	U	SMPL
M2364-02MS - 1	AST2-COPR4-1MS	14592	3.8094	-	7470A	PPB	13 May 2021 15:22:20	U	SMPL
M2364-02MSD - 1	AST2-COPR4-1MSD	14504	3.7863	-	7470A	PPB	13 May 2021 15:24:35	U	SMPL
PB136374TB - 1	PB136317TB	-81	-0.0349	-	7470A	PPB	13 May 2021 15:26:51	U	SMPL
M2364-02LX5 - 1		16	-0.0095	-	7470A	PPB	13 May 2021 15:29:07	U	SMPL
M2364-02A - 1		14312	3.7360	-	7470A	PPB	13 May 2021 15:31:22	U	SMPL
CCV76 - 1	CCV76	18486	4.8296	-	7470A	PPB	13 May 2021 15:33:39	U	SMPL
CCB76 - 1	CCB76	-96	-0.0389	-	7470A	PPB	13 May 2021 15:35:55	U	SMPL