

LB114536


7470A

INSTRUMENT ID: CV1

Linear

μ Abs.:

32213

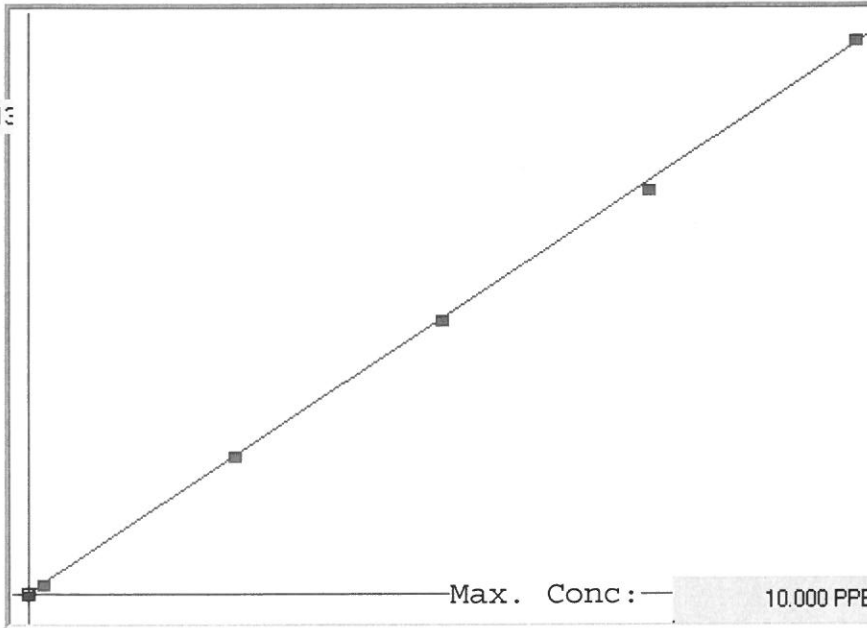

A= 0.0000e+000

B= 3.1315e-004

C= -8.4774e-003

Rho= 0.9998533

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.002	0.002	35	0.000	35					-
0.2	0.200	0.199	-0.001	663	0.0 %	663					-1
2.5	2.500	2.536	0.036	8127	0.0 %	8127					1
5.0	5.000	5.011	0.011	16028	0.0 %	16028					0
7.5	7.500	7.372	-0.128	23570	0.0 %	23570					-2
10.0	10.000	10.079	0.079	32213	0.0 %	32213					1

LB114536 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 19 May 2021 11:33:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	35	-	0.0000	7470A	PPB	19 May 2021 11:45:38	S	Std
0.2 - 1	50.2	663	-	0.2000	7470A	PPB	19 May 2021 11:47:54	S	Std
2.5 - 1	52.5	8127	-	2.5000	7470A	PPB	19 May 2021 11:50:11	S	Std
5.0 - 1	55	16028	-	5.0000	7470A	PPB	19 May 2021 11:52:28	S	Std
7.5 - 1	57.5	23570	-	7.5000	7470A	PPB	19 May 2021 11:54:44	S	Std
10.0 - 1	510	32213	-	10.0000	7470A	PPB	19 May 2021 11:57:00	S	Std
ICV33 - 1	ICV33	11785	3.6820	-	7470A	PPB	19 May 2021 11:59:51	U	SMPL
ICB33 - 1	ICB33	-92	-0.0373	-	7470A	PPB	19 May 2021 12:02:05	U	SMPL
CCV25 - 1	CCV25	15411	4.8174	-	7470A	PPB	19 May 2021 12:04:20	U	SMPL
CCB25 - 1	CCB25	-82	-0.0342	-	7470A	PPB	19 May 2021 12:06:34	U	SMPL
CRA - 1	CRA	603	0.1803	-	7470A	PPB	19 May 2021 12:08:50	U	SMPL
HighStd - 1	HighStd	29793	9.3211	-	7470A	PPB	19 May 2021 12:11:04	U	SMPL
ChkStd - 1	ChkStd	19783	6.1865	-	7470A	PPB	19 May 2021 12:18:37	U	SMPL
M2405-05 - 1	BUR-1022	-9	-0.0113	-	7470A	PPB	19 May 2021 12:45:27	U	SMPL
M2405-05DUP - 1	BUR-1022DUP	101	0.0232	-	7470A	PPB	19 May 2021 12:50:36	U	SMPL
M2405-05MS - 1	BUR-1022MS	12479	3.8993	-	7470A	PPB	19 May 2021 12:55:31	U	SMPL
M2405-05MSD - 1	BUR-1022MSD	12536	3.9171	-	7470A	PPB	19 May 2021 12:57:50	U	SMPL
M2440-01 - 1	TOTE-1	47748	14.9436	-	7470A	PPB	19 May 2021 13:00:05	U	SMPL
CCV26 - 1	CCV26	15500	4.8453	-	7470A	PPB	19 May 2021 13:07:27	U	SMPL
CCB26 - 1	CCB26	75	0.0150	-	7470A	PPB	19 May 2021 13:09:41	U	SMPL
PB136524BL - 1	PBW	223	0.0614	-	7470A	PPB	19 May 2021 13:17:06	U	SMPL
PB136524BS - 1	LCSW	11960	3.7368	-	7470A	PPB	19 May 2021 13:21:57	U	SMPL
M2405-05LX5 - 1		21	-0.0019	-	7470A	PPB	19 May 2021 13:35:07	U	SMPL
M2405-05A - 1		13450	4.2033	-	7470A	PPB	19 May 2021 13:37:22	U	SMPL
M2440-01DLX5 - 1		9127	2.8496	-	7470A	PPB	19 May 2021 13:39:38	U	SMPL
CCV27 - 1	CCV27	15422	4.8209	-	7470A	PPB	19 May 2021 13:41:54	U	SMPL
CCB27 - 1	CCB27	340	0.0980	-	7470A	PPB	19 May 2021 13:46:38	U	SMPL