


LB114567

7471B

INSTRUMENT ID: CV1

 μ Abs.:

48339

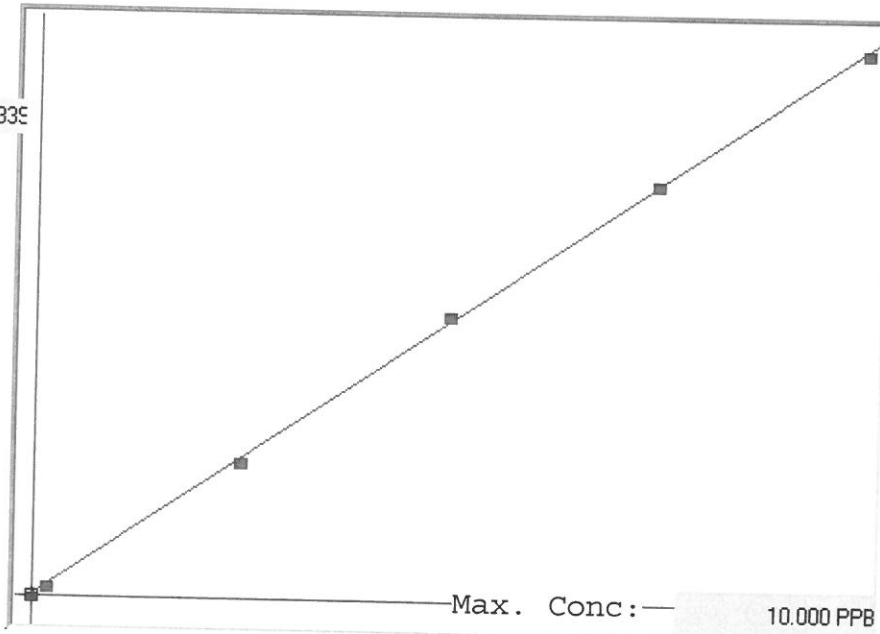

Linear

A= 0.0000e+000

B= 2.0609e-004

C= -2.6895e-002

Rho= 0.9998778

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.001	0.001	133	0.000	133					-
0.2	0.200	0.174	-0.026	975	0.0 %	975					-13
2.5	2.500	2.453	-0.047	12035	0.0 %	12035					-2
5.0	5.000	5.111	0.111	24929	0.0 %	24929					2
7.5	7.500	7.526	0.026	36648	0.0 %	36648					0
10.0	10.000	9.935	-0.065	48339	0.0 %	48339					-1

LB114567 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 20 May 2021 12:04:41

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	133	-	0.0007471B	PPB	20 May 2021 12:13:00	S	Std
0.2 - 1	50.2	975	-	0.20007471B	PPB	20 May 2021 12:15:17	S	Std
2.5 - 1	52.5	12035	-	2.50007471B	PPB	20 May 2021 12:17:34	S	Std
5.0 - 1	55	24929	-	5.00007471B	PPB	20 May 2021 12:19:51	S	Std
7.5 - 1	57.5	36648	-	7.50007471B	PPB	20 May 2021 12:22:07	S	Std
10.0 - 1	59	48339	-	10.00007471B	PPB	20 May 2021 12:24:23	S	Std
ICV35 - 1	ICV35	19126	3.9148	-7471B	PPB	20 May 2021 12:27:16	U	SMPL
ICB35 - 1	ICB35	-124	-0.0525	-7471B	PPB	20 May 2021 12:29:31	U	SMPL
CCV34 - 1	CCV34	24943	5.1136	-7471B	PPB	20 May 2021 12:31:47	U	SMPL
CCB34 - 1	CCB34	-143	-0.0564	-7471B	PPB	20 May 2021 12:34:02	U	SMPL
CRA - 1	CRA	953	0.1695	-7471B	PPB	20 May 2021 12:36:18	U	SMPL
HighStd - 1	HighStd	47855	9.8356	-7471B	PPB	20 May 2021 12:38:33	U	SMPL
ChkStd - 1	ChkStd	34384	7.0593	-7471B	PPB	20 May 2021 12:40:49	U	SMPL
PB136535BL - 1	PBS	-166	-0.0611	-7471B	PPB	20 May 2021 12:43:06	U	SMPL
PB136535BS - 1	LCSS	18027	3.6883	-7471B	PPB	20 May 2021 12:45:23	U	SMPL
M2437-02 - 1	TP-1	85688	17.6326	-7471B	PPB	20 May 2021 12:47:39	U	SMPL
M2437-05 - 1	TP-2	26396	5.4131	-7471B	PPB	20 May 2021 12:49:57	U	SMPL
M2437-08 - 1	TP-3	150465	30.9826	-7471B	PPB	20 May 2021 12:52:16	U	SMPL
M2438-01 - 1	PL-02-051821	84	-0.0096	-7471B	PPB	20 May 2021 12:54:34	U	SMPL
M2439-01 - 1	RO-72-11939	1202	0.2208	-7471B	PPB	20 May 2021 12:56:52	U	SMPL
CCV35 - 1	CCV35	24833	5.0910	-7471B	PPB	20 May 2021 12:59:07	U	SMPL
CCB35 - 1	CCB35	-168	-0.0615	-7471B	PPB	20 May 2021 13:01:22	U	SMPL
M2439-03 - 1	RO-282	2938	0.5786	-7471B	PPB	20 May 2021 13:03:39	U	SMPL
M2439-03DUP - 1	RO-282DUP	2916	0.5741	-7471B	PPB	20 May 2021 13:05:53	U	SMPL
M2439-03MS - 1	RO-282MS	22186	4.5454	-7471B	PPB	20 May 2021 13:08:08	U	SMPL
M2439-03MSD - 1	RO-282MSD	21567	4.4179	-7471B	PPB	20 May 2021 13:10:24	U	SMPL
M2448-01 - 1	HD-01-051821	6800	1.3745	-7471B	PPB	20 May 2021 13:12:40	U	SMPL
M2449-01 - 1	TOP-SOIL-COMPOSITE-PILE-3	4688	0.9393	-7471B	PPB	20 May 2021 13:14:57	U	SMPL
M2457-02 - 1	TP-4	69370	14.2696	-7471B	PPB	20 May 2021 13:17:13	U	SMPL
M2462-01 - 1	WATER-MAIN-BREAK-SOIL	1135	0.2070	-7471B	PPB	20 May 2021 13:19:30	U	SMPL
M2468-01 - 1	1-5-TP	1616	0.3061	-7471B	PPB	20 May 2021 13:21:49	U	SMPL
CCV36 - 1	CCV36	24376	4.9968	-7471B	PPB	20 May 2021 13:24:04	U	SMPL
CCB36 - 1	CCB36	-112	-0.0500	-7471B	PPB	20 May 2021 13:26:19	U	SMPL
M2439-03LX5 - 1		605	0.0978	-7471B	PPB	20 May 2021 13:28:36	U	SMPL
M2439-03A - 1		22377	4.5848	-7471B	PPB	20 May 2021 13:30:51	U	SMPL
M2437-02DLX5 - 1		17874	3.6568	-7471B	PPB	20 May 2021 13:33:07	U	SMPL
M2437-08DLX5 - 1		31776	6.5219	-7471B	PPB	20 May 2021 13:35:24	U	SMPL
M2457-02DLX5 - 1		13742	2.8052	-7471B	PPB	20 May 2021 13:44:15	U	SMPL
CCV37 - 1	CCV37	24338	4.9890	-7471B	PPB	20 May 2021 13:46:34	U	SMPL
CCB37 - 1	CCB37	-92	-0.0459	-7471B	PPB	20 May 2021 13:48:50	U	SMPL