

LB114586


7470A

INSTRUMENT ID: EV2

Linear

μ Abs.:

36793

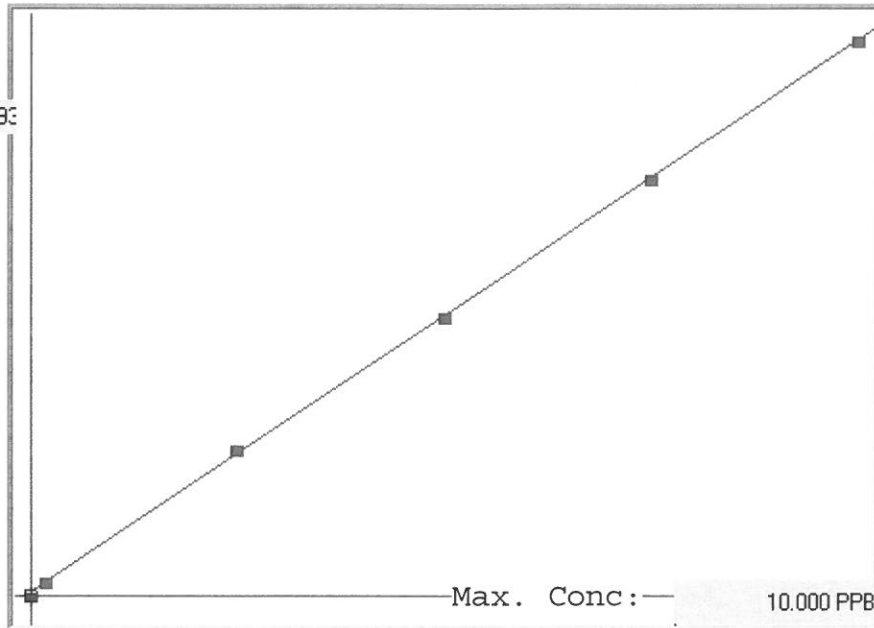

A= 0.0000e+000

B= 2.7311e-004

C= -6.9291e-002

Rho= 0.9999418

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.044	-0.044	94	0.000	94					
0.2	0.200	0.185	-0.015	930	0.0 %	930					-8
2.5	2.500	2.583	0.083	9711	0.0 %	9711					3
5.0	5.000	4.993	-0.007	18535	0.0 %	18535					0
7.5	7.500	7.504	0.004	27729	0.0 %	27729					0
10.0	10.000	9.979	-0.021	36793	0.0 %	36793					0

LB114586 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 21 May 2021 14:30:02					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	94	-	0.0000	7470A	PPB	21 May 2021 14:33:23	S	Std
0.2 - 1	50.2	930	-	0.2000	7470A	PPB	21 May 2021 14:35:40	S	Std
2.5 - 1	52.5	9711	-	2.5000	7470A	PPB	21 May 2021 14:37:57	S	Std
5.0 - 1	55	18535	-	5.0000	7470A	PPB	21 May 2021 14:40:14	S	Std
7.5 - 1	57.5	27729	-	7.5000	7470A	PPB	21 May 2021 14:45:22	S	Std
10.0 - 1	510	36793	-	10.0000	7470A	PPB	21 May 2021 14:50:17	S	Std
ICV36 - 1	ICV36	14654	3.9329	-7470A	PPB	PPB	21 May 2021 14:52:59	U	SMPL
ICB36 - 1	ICB36	-96	-0.0955	-7470A	PPB	PPB	21 May 2021 14:55:16	U	SMPL
CCV47 - 1	CCV47	18285	4.9246	-7470A	PPB	PPB	21 May 2021 14:57:31	U	SMPL
CCB47 - 1	CCB47	-103	-0.0974	-7470A	PPB	PPB	21 May 2021 14:59:46	U	SMPL
CRA - 1	CRA	894	0.1749	-7470A	PPB	PPB	21 May 2021 15:02:02	U	SMPL
HighStd - 1	HighStd	36487	9.8958	-7470A	PPB	PPB	21 May 2021 15:06:48	U	SMPL
ChkStd - 1	ChkStd	25821	6.9827	-7470A	PPB	PPB	21 May 2021 15:09:02	U	SMPL
PB136586BL - 1	PBW	-4	-0.0704	-7470A	PPB	PPB	21 May 2021 15:11:20	U	SMPL
PB136586BS - 1	LCSW	14831	3.9812	-7470A	PPB	PPB	21 May 2021 15:13:36	U	SMPL
M2457-03 - 1	TP-4	66	-0.0513	-7470A	PPB	PPB	21 May 2021 15:15:52	U	SMPL
M2467-02 - 1	IDW-BR3-SO-051921	171	-0.0226	-7470A	PPB	PPB	21 May 2021 15:18:08	U	SMPL
M2467-02DUP - 1	IDW-BR3-SO-051921DUP	157	-0.0264	-7470A	PPB	PPB	21 May 2021 15:20:25	U	SMPL
M2467-02MS - 1	IDW-BR3-SO-051921MS	13150	3.5221	-7470A	PPB	PPB	21 May 2021 15:22:42	U	SMPL
M2467-02MSD - 1	IDW-BR3-SO-051921MSD	13132	3.5172	-7470A	PPB	PPB	21 May 2021 15:24:58	U	SMPL
CCV48 - 1	CCV48	18357	4.9442	-7470A	PPB	PPB	21 May 2021 15:27:15	U	SMPL
CCB48 - 1	CCB48	-122	-0.1026	-7470A	PPB	PPB	21 May 2021 15:29:31	U	SMPL
PB136586TB - 1	PB136565TB	174	-0.0218	-7470A	PPB	PPB	21 May 2021 15:31:46	U	SMPL
M2467-02LX5 - 1		45	-0.0570	-7470A	PPB	PPB	21 May 2021 15:34:01	U	SMPL
M2467-02A - 1		15061	4.0441	-7470A	PPB	PPB	21 May 2021 15:36:17	U	SMPL
CCV49 - 1	CCV49	18362	4.9456	-7470A	PPB	PPB	21 May 2021 15:41:01	U	SMPL
CCB49 - 1	CCB49	-110	-0.0993	-7470A	PPB	PPB	21 May 2021 15:43:16	U	SMPL