


LB114626

7471B

INSTRUMENT ID: CV2

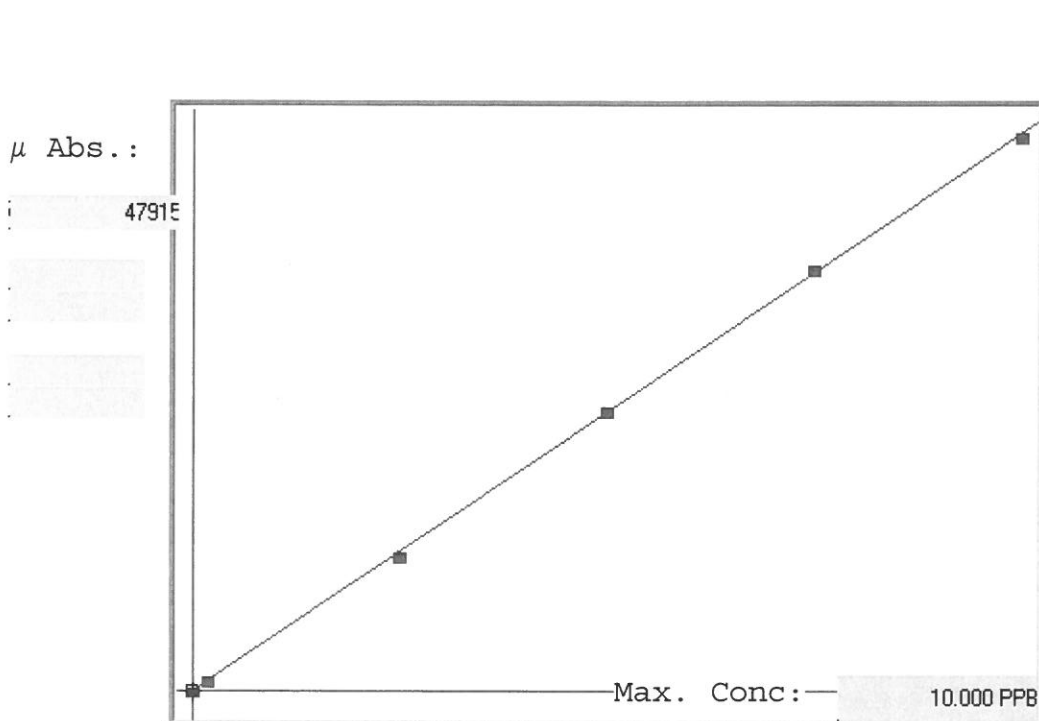

Linear

A= 0.0000e+000

B= 2.0713e-004

C= 4.0578e-003

Rho= 0.9998660

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	u/v)
0.0	0.000	0.010	0.010	30	0.000	30					
0.2	0.200	0.210	0.010	993	0.0 %	993					5
2.5	2.500	2.419	-0.081	11658	0.0 %	11658					-3
5.0	5.000	5.041	0.041	24316	0.0 %	24316					1
7.5	7.500	7.592	0.092	36631	0.0 %	36631					1
10.0	10.000	9.929	-0.071	47915	0.0 %	47915					-1

LB114626 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 25 May 2021 13:52:16

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	30	-	0.0000	7471B	PPB	25 May 2021 13:54:40	S	Std
0.2 - 1	50.2	993	-	0.2000	7471B	PPB	25 May 2021 13:56:57	S	Std
2.5 - 1	52.5	11658	-	2.5000	7471B	PPB	25 May 2021 13:59:13	S	Std
5.0 - 1	55	24316	-	5.0000	7471B	PPB	25 May 2021 14:01:30	S	Std
7.5 - 1	57.5	36631	-	7.5000	7471B	PPB	25 May 2021 14:03:46	S	Std
10.0 - 1	510	47915	-	10.0000	7471B	PPB	25 May 2021 14:06:02	S	Std
ICV39 - 1	ICV39	19271	3.9957	-	7471B	PPB	25 May 2021 14:08:48	U	SMPL
ICB39 - 1	ICB39	-122	-0.0212	-	7471B	PPB	25 May 2021 14:11:03	U	SMPL
CCV63 - 1	CCV63	24447	5.0679	-	7471B	PPB	25 May 2021 14:13:18	U	SMPL
CCB63 - 1	CCB63	-147	-0.0264	-	7471B	PPB	25 May 2021 14:15:33	U	SMPL
CRA - 1	CRA	999	0.2110	-	7471B	PPB	25 May 2021 14:17:48	U	SMPL
HighStd - 1	HighStd	48068	9.9606	-	7471B	PPB	25 May 2021 14:20:03	U	SMPL
ChkStd - 1	ChkStd	34469	7.1437	-	7471B	PPB	25 May 2021 14:22:18	U	SMPL
PB136641BL - 1	PBS	-173	-0.0318	-	7471B	PPB	25 May 2021 14:24:35	U	SMPL
PB136641BS - 1	LCSS	20250	4.1985	-	7471B	PPB	25 May 2021 14:26:52	U	SMPL
M2214-11 - 1	PT-MET-SOIL	686956	HIGH	-	7471B	PPB	25 May 2021 14:29:08	X	
M2500-01 - 1	NB-08-052421	1279	0.2690	-	7471B	PPB	25 May 2021 14:33:53	U	SMPL
M2500-01DUP - 1	NB-08-052421DUP	1070	0.2257	-	7471B	PPB	25 May 2021 14:36:09	U	SMPL
M2500-01MS - 1	NB-08-052421MS	21819	4.5235	-	7471B	PPB	25 May 2021 14:38:27	U	SMPL
M2500-01MSD - 1	NB-08-052421MSD	21902	4.5407	-	7471B	PPB	25 May 2021 14:40:42	U	SMPL
CCV64 - 1	CCV64	23859	4.9461	-	7471B	PPB	25 May 2021 14:42:58	U	SMPL
CCB64 - 1	CCB64	-149	-0.0268	-	7471B	PPB	25 May 2021 14:45:14	U	SMPL
M2502-01 - 1	SA-01-052421	1570	0.3293	-	7471B	PPB	25 May 2021 14:47:30	U	SMPL
M2503-01 - 1	OK-01-052421	4818	1.0020	-	7471B	PPB	25 May 2021 14:49:45	U	SMPL
M2500-01LX5 - 1		383	0.0834	-	7471B	PPB	25 May 2021 15:00:02	U	SMPL
M2500-01A - 1		21488	4.4549	-	7471B	PPB	25 May 2021 15:02:17	U	SMPL
M2214-11DLX10 - 1	PT-MET-SOIL	141126	29.2360	-	7471B	PPB	25 May 2021 15:06:52	U	SMPL
CCV65 - 1	CCV65	23215	4.8127	-	7471B	PPB	25 May 2021 15:11:32	U	SMPL
CCB65 - 1	CCB65	-224	-0.0423	-	7471B	PPB	25 May 2021 15:13:50	U	SMPL
M2214-11DL2X50 - 1	PT-MET-SOIL	28917	5.9937	-	7471B	PPB	25 May 2021 15:23:20	U	SMPL
CCV66 - 1	CCV66	23220	4.8137	-	7471B	PPB	25 May 2021 15:25:36	U	SMPL
CCB66 - 1	CCB66	-149	-0.0268	-	7471B	PPB	25 May 2021 15:27:52	U	SMPL