

IC-7
300-0
6/02/2021
AM


Clear table

ident	concentra tion F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-05-24_	5/24/21 15:19		AM/AP
STD2	0.4460	0.6680	0.6660	2.2150	0.5670	0.9150	3.4840	_2021-05-24_	5/24/21 15:49		AM/AP
STD3	0.7810	1.2030	1.1980	4.0470	1.0110	2.0040	6.0490	_2021-05-24_	5/24/21 16:18		AM/AP
STD4	1.0510	1.5020	1.4870	4.9860	1.2460	2.5230	7.4680	_2021-05-24_	5/24/21 16:48		AM/AP
STD5	1.9550	2.9260	2.9460	9.7370	2.4220	5.1220	14.4590	_2021-05-24_	5/24/21 17:17		AM/AP
STD6	3.8460	5.9060	5.9340	19.7170	4.9170	9.9300	29.4710	_2021-05-24_	5/24/21 17:47		AM/AP
STD7	5.1210	7.5940	7.5700	25.2980	6.3370	12.5060	38.0690	_2021-05-24_	5/24/21 18:17		AM/AP
ICV	1.9940	2.9230	2.9530	9.7360	2.4220	5.3240	14.4740	_2021-05-24_	5/24/21 18:46		AM/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-05-24_	5/24/21 19:16		AM/AP
CCV	2.0260	2.8330	2.8110	9.2980	2.3330	4.5620	14.0290	_2021-06-01_	6/1/21 9:43		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-06-01_	6/1/21 10:17		AM/AP
LB114681BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-06-01_	6/1/21 10:47		AM/AP
LB114681BSW	1.9420	2.8110	2.8360	9.2870	2.3240	4.8510	13.9340	_2021-06-01_	6/1/21 11:16		AM/AP
M2262-07	0.2550	0.3570	0.3890	1.3160	0.3420	0.2110	2.1580	_2021-06-01_	6/1/21 11:45		AM/AP
M2262-08	0.4560	0.6440	0.6810	2.2570	0.5770	0.9680	3.5050	_2021-06-01_	6/1/21 12:43		AM/AP
CCV	1.9870	2.8370	2.8670	9.4370	2.3440	5.2150	14.0780	_2021-06-01_	6/1/21 13:17		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2021-06-01_	6/1/21 14:01		AM/AP

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-052421.mtw
 Equation: $Q = 0.078782 \cdot A + 1.71235$
 RSD: 4.844 %
 Correlation coefficient: 0.998720

IC-2
 5/25/2021
 AM

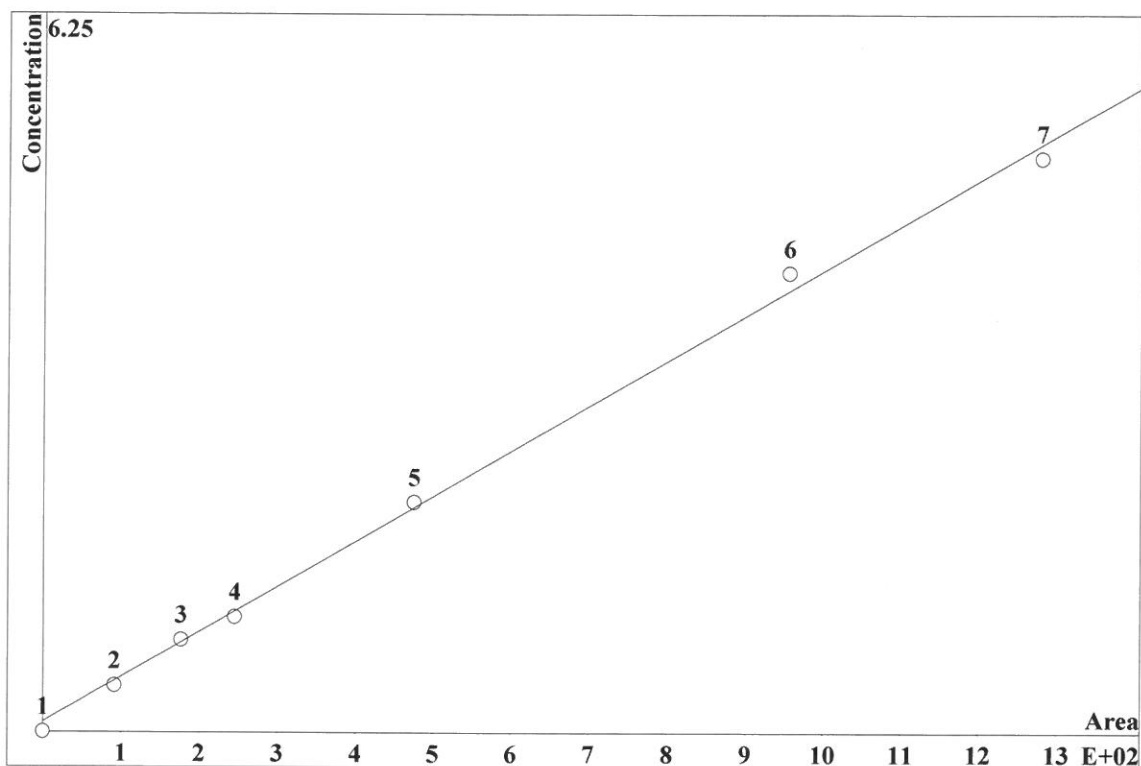


K3 = 0 K2 = 0 K1 = 0.078782 K0 = 1.71235
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.086	91.45	0.4	20	5.75		
3	6.052	176.6	0.8	20	5.75		
4	8.531	245	1	20	5.75		
5	18.47	474.5	2	20	5.75		
6	36.12	954.7	4	20	5.75		
7	48.28	1278	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-052421.mtw
 Equation: $Q = 0.115267 \cdot A + 1.56543$
 RSD: 2.529 %
 Correlation coefficient: 0.999651

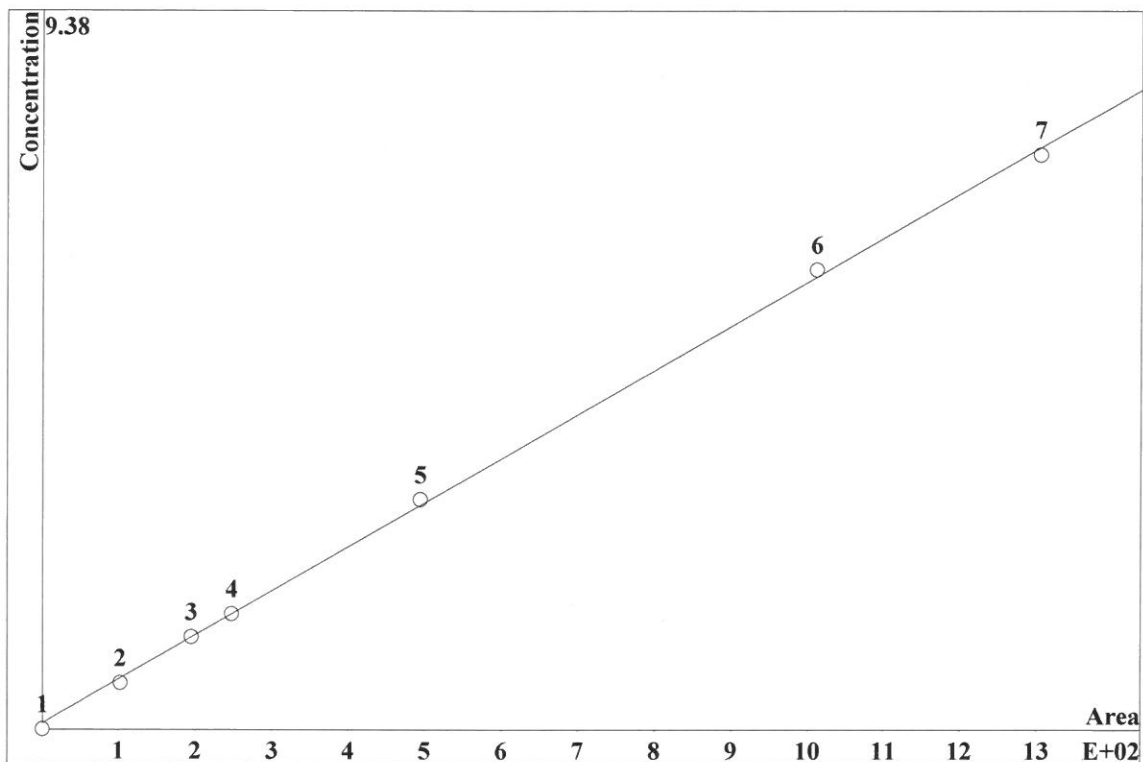


K3 = 0 K2 = 0 K1 = 0.115267 K0 = 1.56543
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.966	102.4	0.6	20	8.834		
3	13.43	195.1	1.2	20	8.834		
4	16.9	247.1	1.5	20	8.834		
5	34.48	494.1	3	20	8.834		
6	72.05	1011	6	20	8.834		
7	92.55	1304	7.5	20	8.834		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-052421.mtw
 Equation: $Q = 0.050927 \cdot A + 2.29171$
 RSD: 1.959 %
 Correlation coefficient: 0.999791

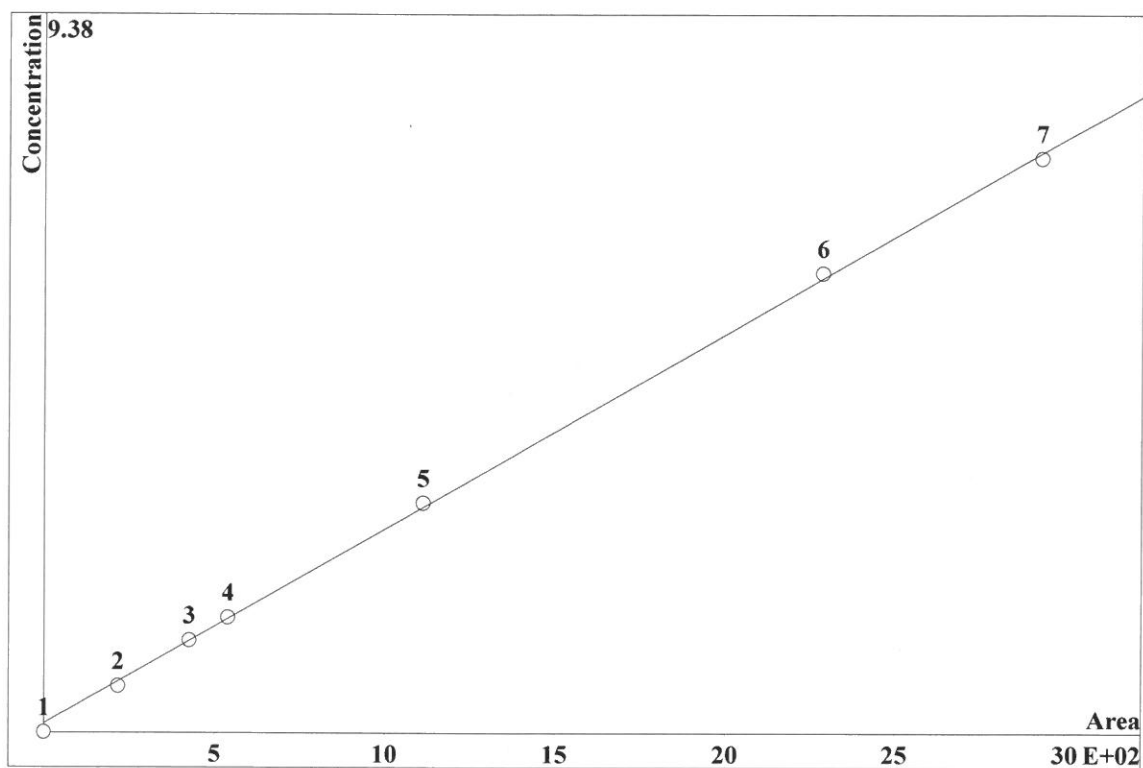


K3 = 0 K2 = 0 K1 = 0.050927 K0 = 2.29171
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	11.19	216.4	0.6	20	10.64	
3	21.88	425.4	1.2	20	10.64	
4	27.74	538.9	1.5	20	10.64	
5	57.32	1112	3	20	10.64	
6	114.9	2285	6	20	10.64	
7	145.7	2928	7.5	20	10.64	

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-052421.mtw
 Equation: $Q = 0.253839 \cdot A + 8.10754$
 RSD: 2.435 %
 Correlation coefficient: 0.999677

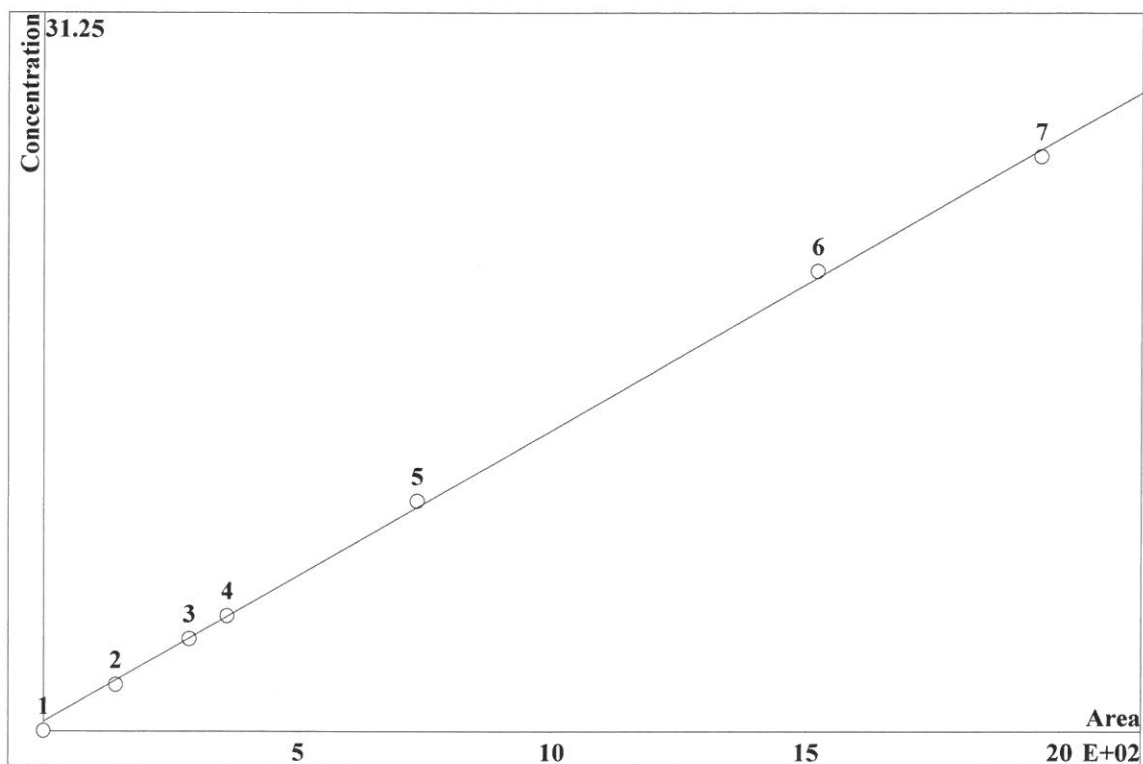


K3 = 0 K2 = 0 K1 = 0.253839 K0 = 8.10754
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.396	142.6	2	20			14
3	14.93	287	4	20			14
4	18.96	360.9	5	20			14
5	39.45	735.2	10	20			14
6	83.1	1522	20	20			14
7	108.6	1961	25	20			14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-052421.mtw
 Equation: $Q = 0.0443329 \cdot A + 2.28914$
 RSD: 2.884 %
 Correlation coefficient: 0.999547

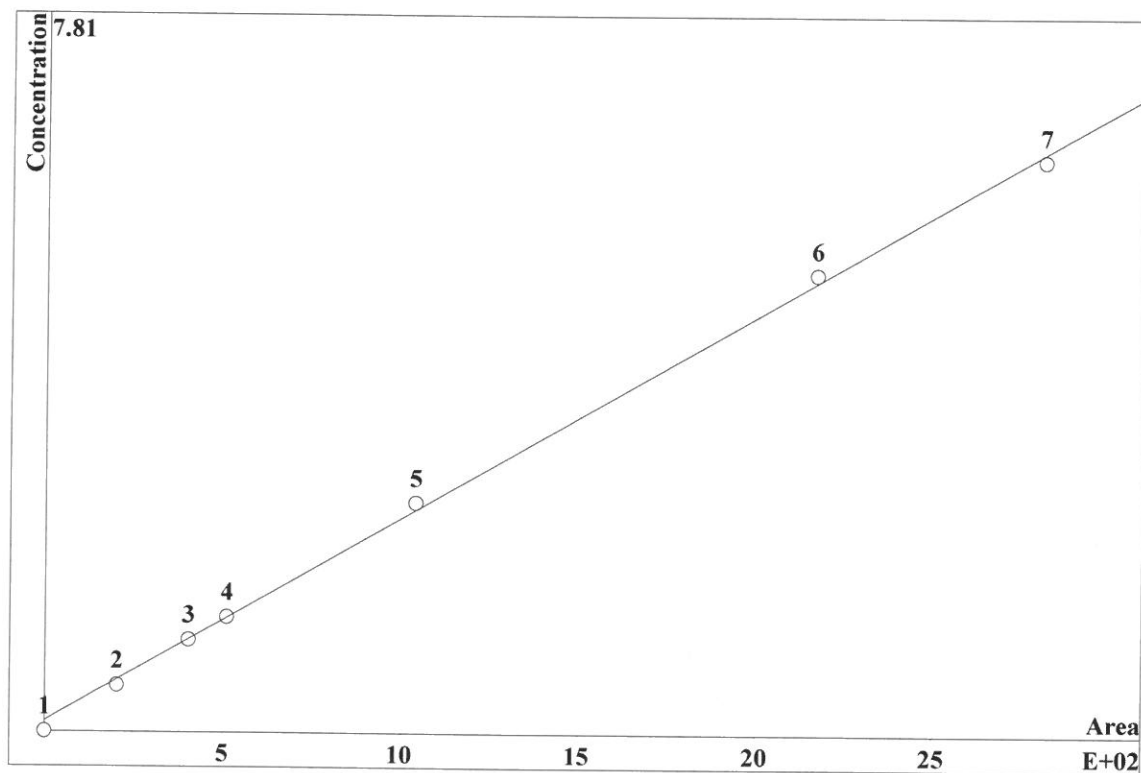


K3 = 0 K2 = 0 K1 = 0.0443329 K0 = 2.28914
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	8.995	204.2	0.5	20	14.79	
3	17.91	404.3	1	20	14.79	
4	22.7	510.5	1.25	20	14.79	
5	46.65	1041	2.5	20	14.79	
6	97.07	2167	5	20	14.79	
7	126.4	2807	6.25	20	14.79	

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-052421.mtw
 Equation: $Q = 0.10127 \cdot A - 11.7243$
 RSD: 1.510 %
 Correlation coefficient: 0.999876

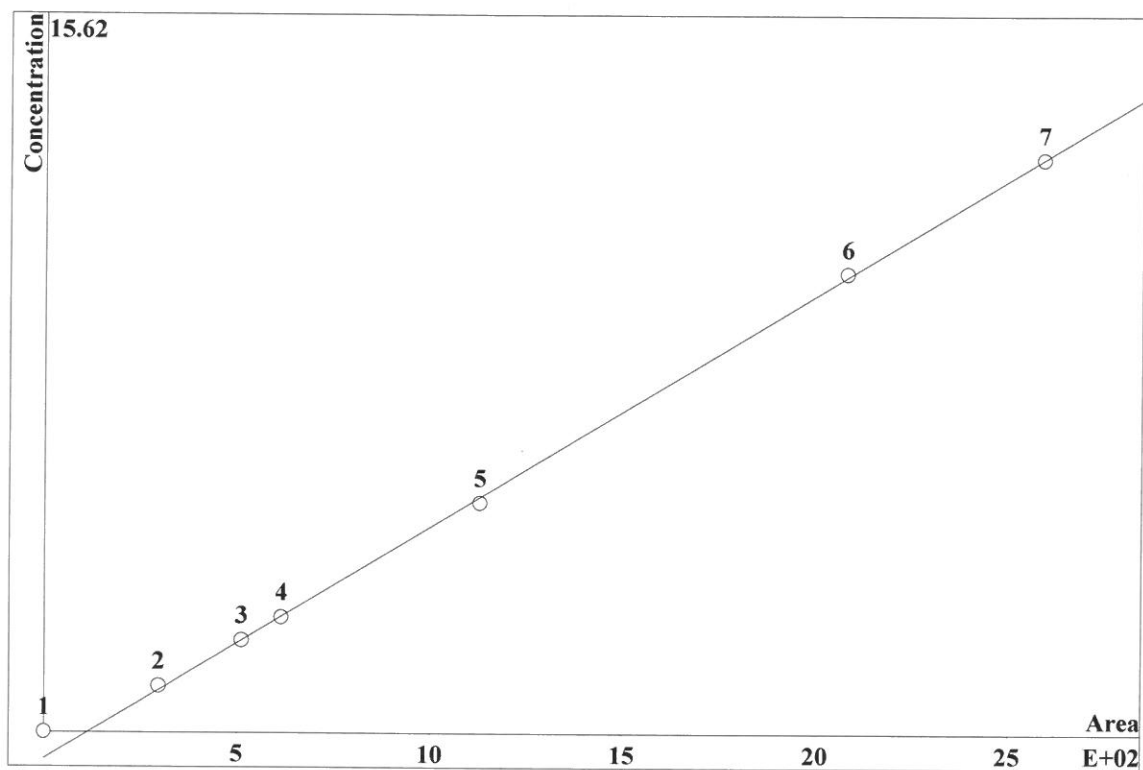


K3 = 0 K2 = 0 K1 = 0.10127 K0 = -11.7243
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.388	296.4	1	20	21.2		
3	13.78	511.5	2	20	21.2		
4	16.53	614.1	2.5	20	21.2		
5	32.57	1127	5	20	21.2		
6	62.84	2077	10	20	21.2		
7	79.04	2586	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-052421.mtw
 Equation: $Q = 0.143282 \cdot A + 15.8948$
 RSD: 3.226 %
 Correlation coefficient: 0.999433

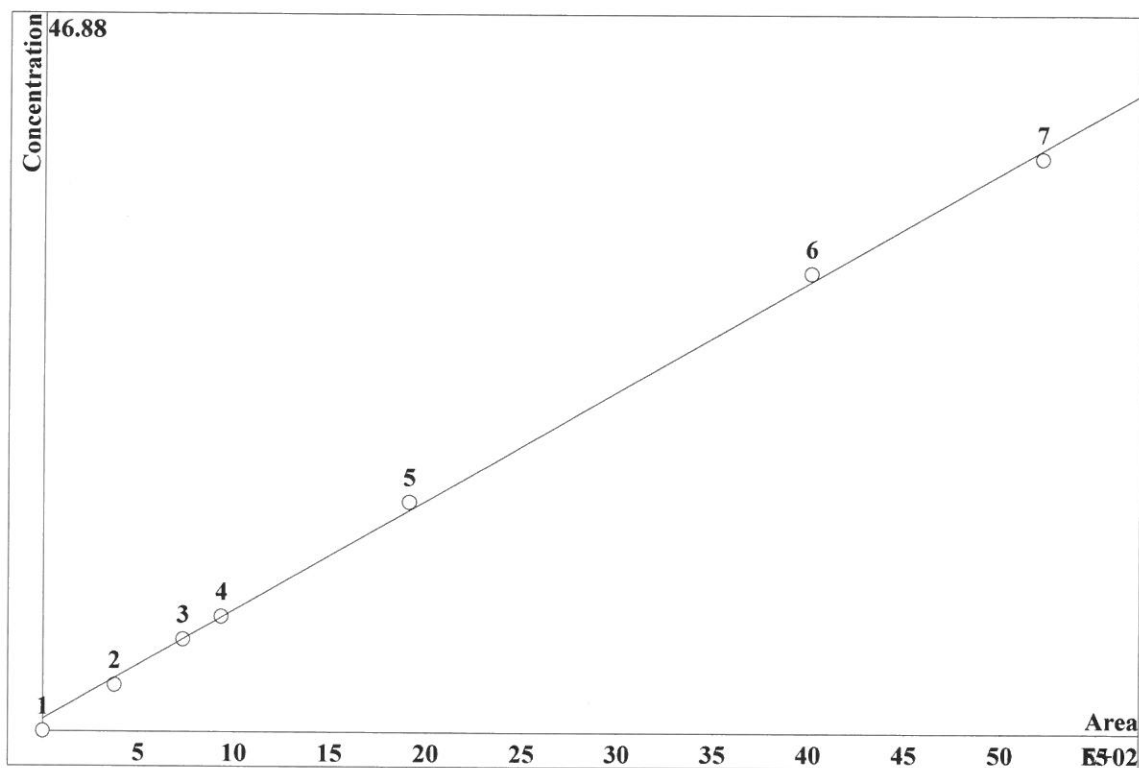

K3 = 0 K2 = 0 K1 = 0.143282 K0 = 15.8948
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	12.97	375.4	3	20	24.73	
3	25.5	733.4	6	20	24.73	
4	32.41	931.4	7.5	20	24.73	
5	67.36	1907	15	20	24.73	
6	142.5	4003	30	20	24.73	
7	186.5	5203	37.5	20	24.73	

Report date: 5/25/2021 2:00:40 PM
Printed by: wet


Ident: STD1
Analysis from: 5/24/2021 3:19:25 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:02 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27031

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

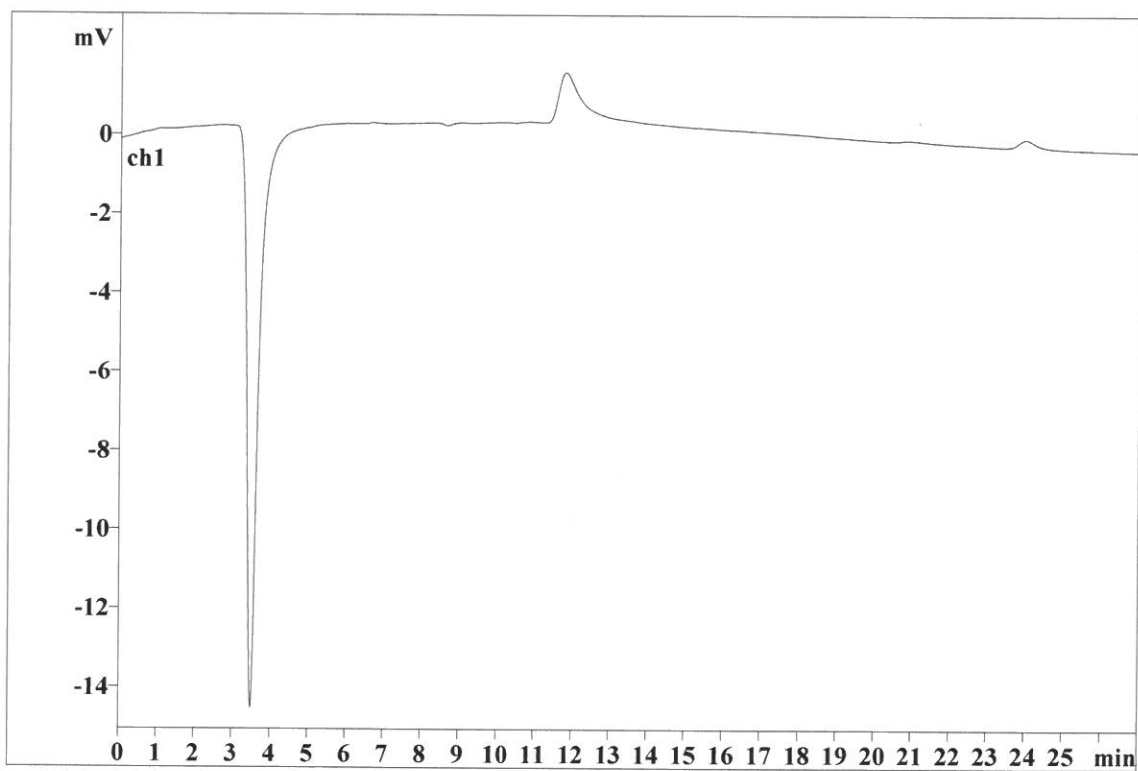

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 5/25/2021 2:00:49 PM
Printed by: wet


Ident: STD2
Analysis from: 5/24/2021 3:49:00 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:02 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27032

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

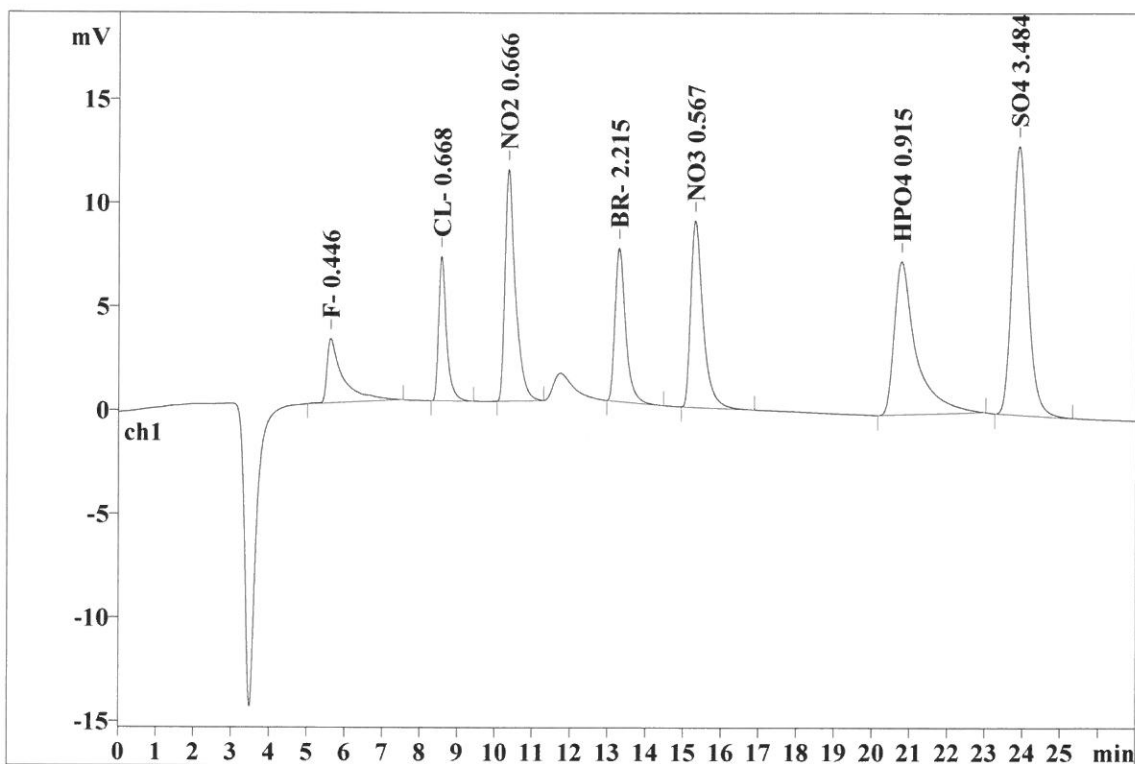

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.349	3.09	5.32	91.449	6.40
2	8.55	0.211	6.96	12.01	102.372	7.17
3	10.33	0.276	11.19	19.29	216.368	15.14
4	13.27	0.282	7.40	12.75	142.559	9.98
5	15.28	0.330	8.99	15.51	204.152	14.29
6	20.75	0.518	7.39	12.74	296.406	20.75
7	23.86	0.434	12.97	22.36	375.366	26.27
7	27.00	0.343	57.98	99.99	1428.673	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/25/2021 2:00:56 PM
Printed by: wet


Ident: STD3
Analysis from: 5/24/2021 4:18:36 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:02 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27033

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

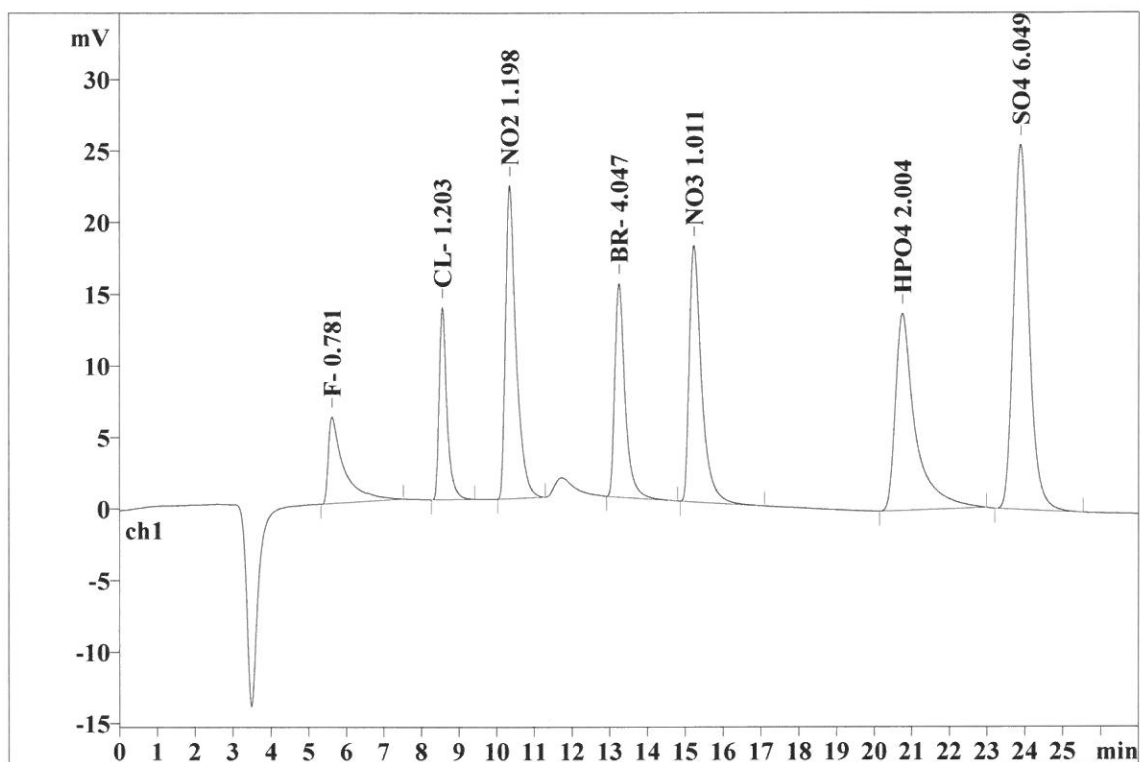

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.356	6.05	5.33	176.591	6.46
2	8.54	0.209	13.43	11.83	195.070	7.14
3	10.32	0.279	21.88	19.28	425.404	15.56
4	13.23	0.278	14.93	13.15	286.955	10.50
5	15.22	0.326	17.91	15.78	404.268	14.79
6	20.73	0.485	13.78	12.14	511.463	18.71
7	23.87	0.430	25.50	22.47	733.401	26.83
7	27.00	0.338	113.46	99.99	2733.151	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/25/2021 2:01:03 PM
Printed by: wet


Ident: STD4
Analysis from: 5/24/2021 4:48:12 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:03 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27034

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

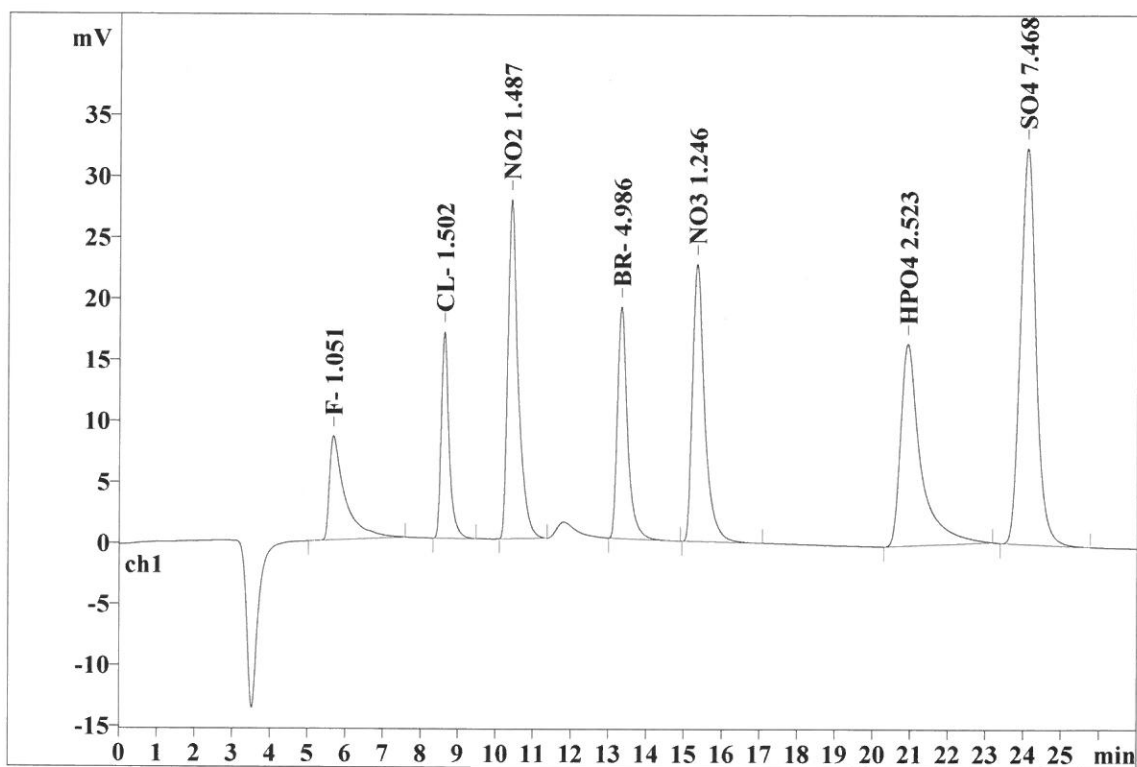

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.67	0.363	8.53	5.93	244.984	7.11
2	8.61	0.211	16.90	11.76	247.115	7.17
3	10.39	0.279	27.74	19.29	538.901	15.63
4	13.31	0.277	18.96	13.18	360.887	10.47
5	15.31	0.327	22.70	15.79	510.502	14.81
6	20.90	0.486	16.53	11.49	614.066	17.81
7	24.06	0.431	32.41	22.54	931.437	27.01
7	27.00	0.339	143.77	100.00	3447.892	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/25/2021 2:01:09 PM
Printed by: wet


Ident: STD5
Analysis from: 5/24/2021 5:17:48 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:03 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27035

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

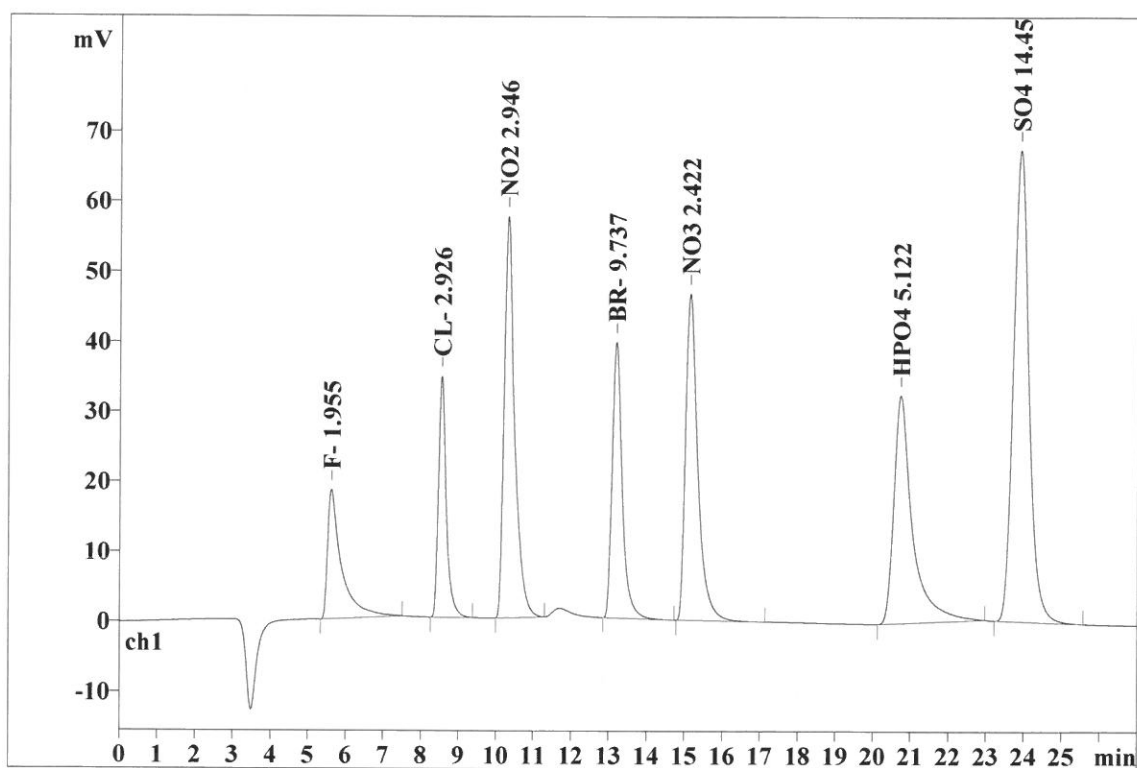

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.321	18.47	6.23	474.547	6.89
2	8.53	0.205	34.48	11.64	494.079	7.17
3	10.28	0.276	57.32	19.35	1111.947	16.13
4	13.17	0.270	39.45	13.31	735.231	10.67
5	15.11	0.323	46.65	15.74	1041.035	15.11
6	20.71	0.460	32.57	10.99	1127.319	16.36
7	23.86	0.423	67.36	22.73	1907.372	27.68
7	27.00	0.325	296.29	100.00	6891.530	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/25/2021 2:01:16 PM
Printed by: wet


Ident: STD6
Analysis from: 5/24/2021 5:47:24 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:03 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27036

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

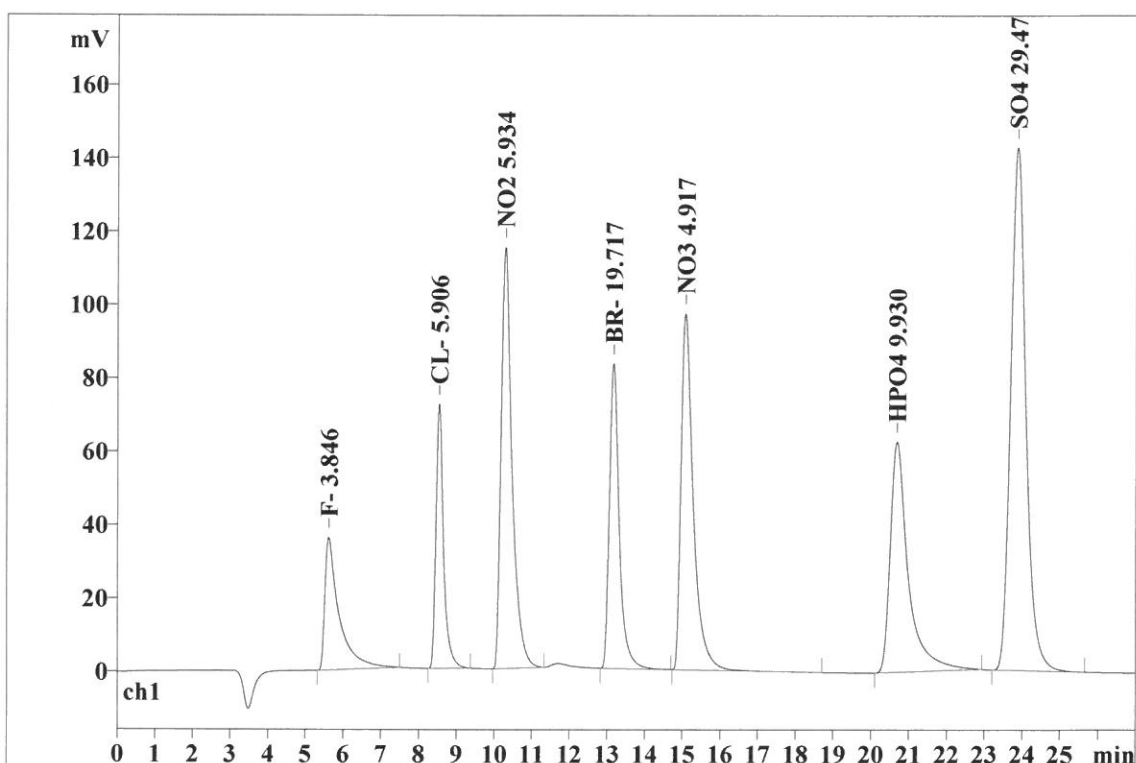

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.336	36.12	5.94	954.662	6.81
2	8.53	0.200	72.05	11.84	1011.236	7.21
3	10.26	0.284	114.87	18.88	2285.250	16.30
4	13.15	0.264	83.09	13.65	1521.555	10.85
5	15.06	0.319	97.06	15.95	2166.645	15.45
6	20.67	0.444	62.84	10.33	2076.930	14.81
7	23.83	0.419	142.53	23.42	4002.834	28.55
7	27.00	0.324	608.58	100.00	14019.112	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/25/2021 2:01:22 PM
Printed by: wet


Ident: STD7
Analysis from: 5/24/2021 6:17:00 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:03 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27037

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

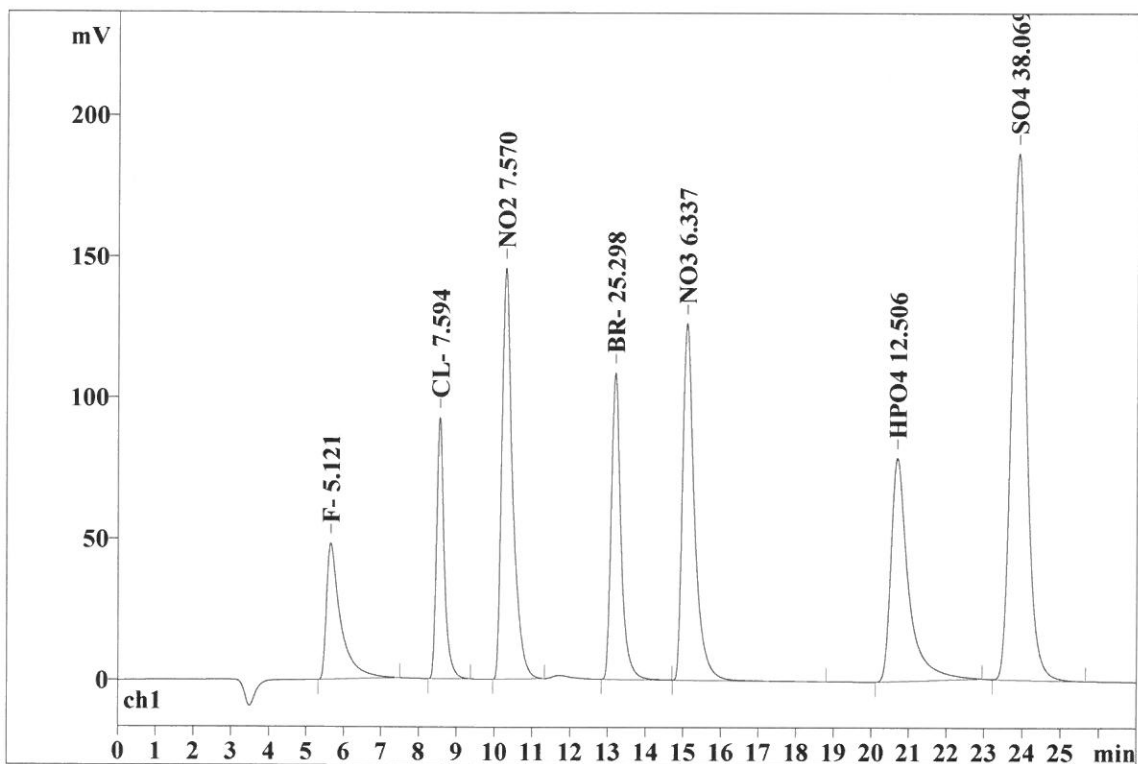

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.352	48.27	6.13	1278.373	7.08
2	8.54	0.202	92.55	11.76	1304.131	7.22
3	10.27	0.291	145.72	18.51	2927.966	16.21
4	13.17	0.262	108.60	13.80	1961.316	10.86
5	15.07	0.319	126.38	16.06	2807.271	15.54
6	20.67	0.443	79.04	10.04	2585.678	14.31
7	23.85	0.418	186.50	23.70	5202.920	28.80
7	27.00	0.327	787.05	100.00	18067.655	100.00

This report has been created by IC Net
METROHM LTD

Date - 5/25/2021

Analyst - AM

Anion Calibration std - relative error calculations, acceptance limit is -30 to 30 for std 2 and -10 to 10 for other std																		
Parameter	TV of std2	Result of std2	% RE std2	TV of std3	Result of std3	% RE std3	TV of std4	Result of std4	% RE std4	TV of std5	Result of std5	% RE std5	TV of std6	Result of std6	% RE std6	TV of std7	Result of std7	% RE std7
F	0.4	0.446	11.5	0.8	0.781	-2.4	1	1.051	5.1	2	1.955	-2.3	4	3.846	-3.9	5	5.121	2.4
CL	0.6	0.668	11.3	1.2	1.203	0.3	1.5	1.502	0.1	3	2.926	-2.5	6	5.906	-1.6	7.5	7.594	1.3
NO2	0.6	0.666	11.0	1.2	1.198	-0.2	1.5	1.487	-0.9	3	2.946	-1.8	6	5.934	-1.1	7.5	7.570	0.9
BR	2	2.215	10.8	4	4.047	1.2	5	4.986	-0.3	10	9.737	-2.6	20	19.717	-1.4	25	25.298	1.2
NO3	0.5	0.567	13.4	1	1.011	1.1	1.25	1.246	-0.3	2.5	2.422	-3.1	5	4.917	-1.7	6.25	6.337	1.4
HPO4	1	0.915	-8.5	2	2.004	0.2	2.5	2.523	0.9	5	5.122	2.4	10	9.930	-0.7	12.5	12.506	0.0
SO4	3	3.484	16.1	6	6.049	0.8	7.5	7.468	-0.4	15	14.459	-3.6	30	29.471	-1.8	37.5	38.069	1.5

05/25/2021
AM

Report date: 5/25/2021 2:01:30 PM
Printed by: wet


Ident: ICV
Analysis from: 5/24/2021 6:46:35 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:03 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27038

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

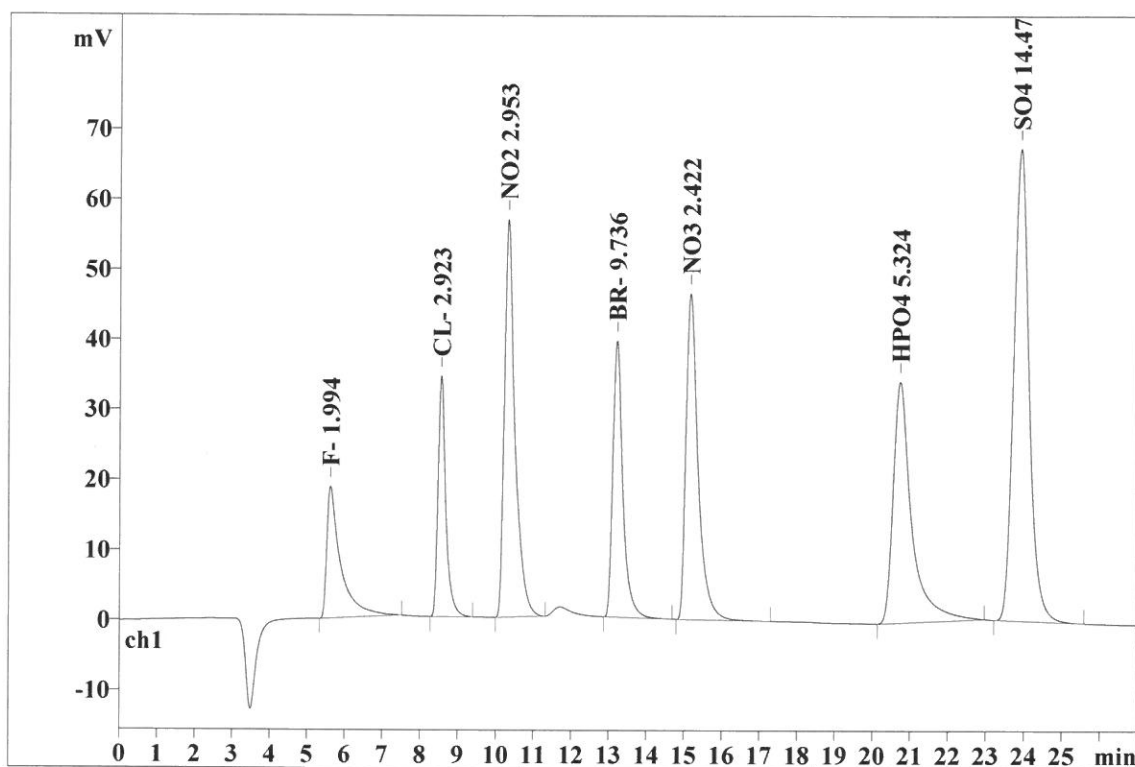

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.324	18.76	6.31	484.509	6.98
2	8.53	0.205	34.31	11.54	493.514	7.11
3	10.29	0.277	56.74	19.08	1114.603	16.05
4	13.19	0.271	39.36	13.24	735.175	10.58
5	15.14	0.324	46.48	15.63	1041.118	14.99
6	20.70	0.454	34.33	11.54	1167.125	16.80
7	23.86	0.424	67.33	22.65	1909.447	27.49
7	27.00	0.326	297.31	100.00	6945.490	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/25/2021 2:01:38 PM
Printed by: wet


Ident: ICB
Analysis from: 5/24/2021 7:16:10 PM
File: _2021-05-24_

Last save: 5/24/2021 9:10:03 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27039

Last save: 5/24/2021 6:14:

SAMPLE:
: AM/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

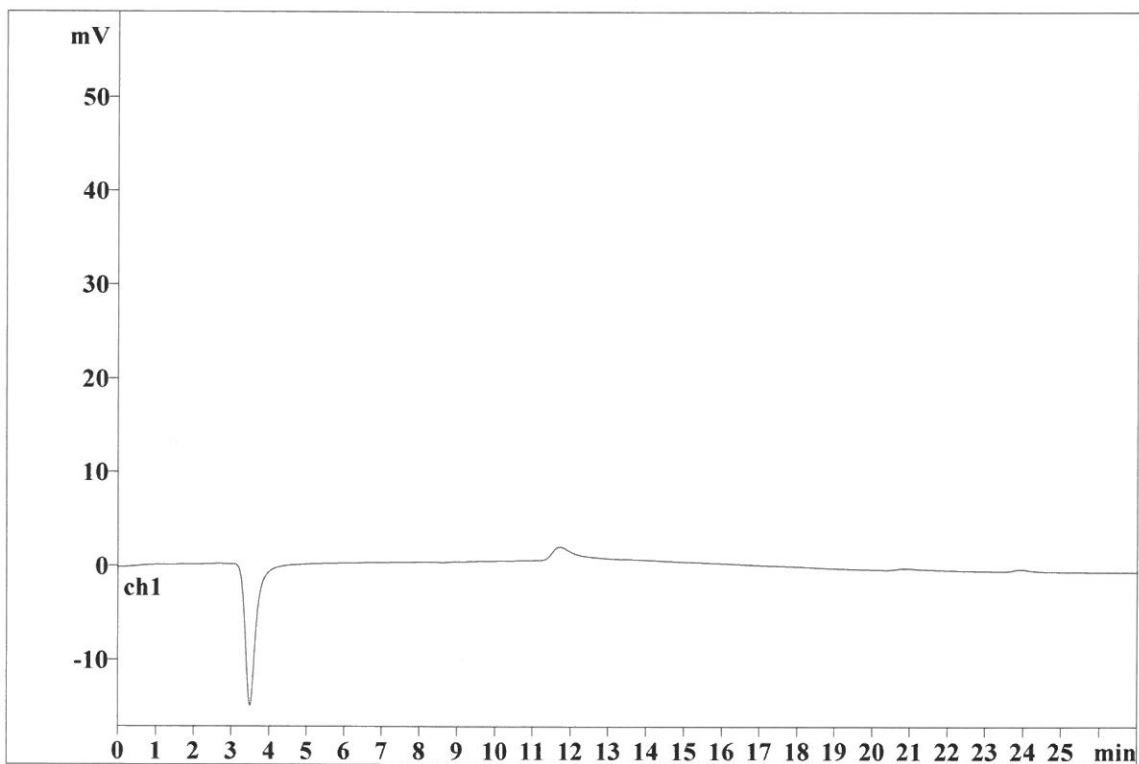

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 6/1/2021 4:33:16 PM
Printed by: wet


Ident: CCV
Analysis from: 6/1/2021 9:43:06 AM
File: 2021-06-01

Last save: 6/1/2021 10:09:36 AM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27148

Last save: 5/27/2021 12:48

SAMPLE:
: AM/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

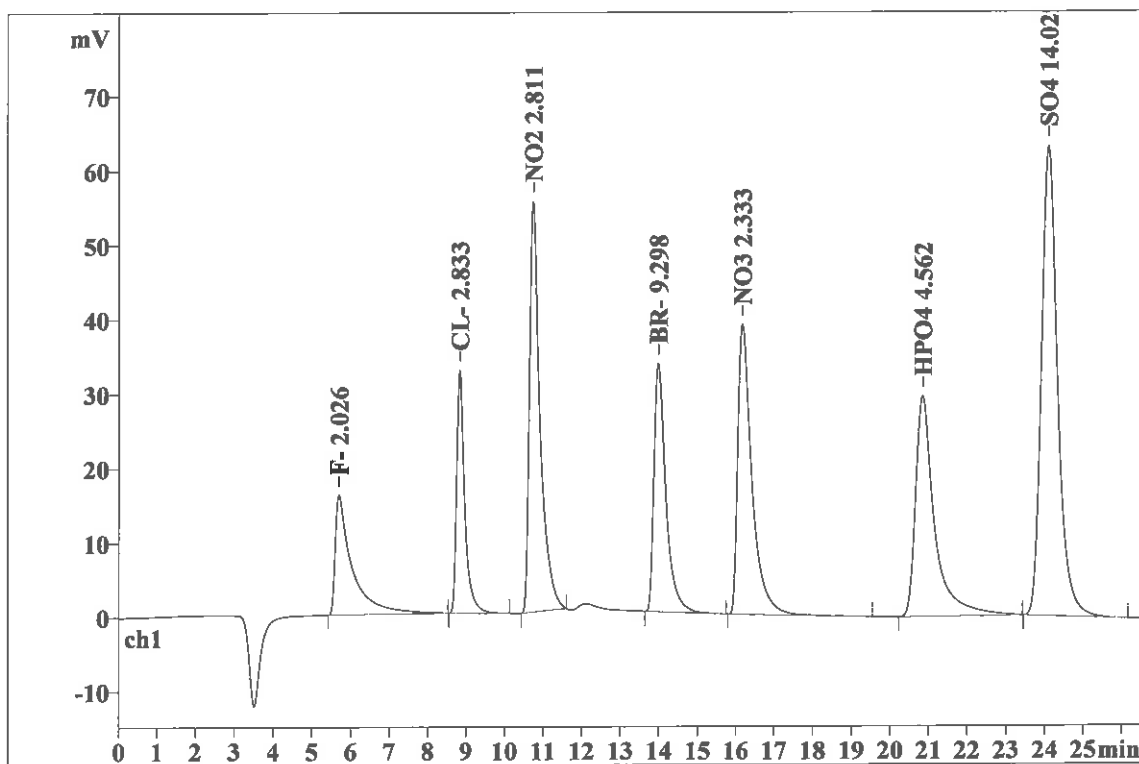

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.360	16.11	5.99	492.560	7.47
2	8.83	0.205	32.63	12.13	477.938	7.25
3	10.74	0.267	55.17	20.51	1059.092	16.06
4	13.99	0.301	33.36	12.40	700.686	10.62
5	16.17	0.364	38.97	14.48	1000.933	15.18
6	20.83	0.453	29.69	11.04	1016.740	15.42
7	24.09	0.433	63.12	23.46	1847.349	28.01
7	26.50	0.340	269.05	100.00	6595.298	100.00

This report has been created by IC Net
METROHM LTD

Report date: 6/1/2021 4:33:25 PM
Printed by: wet


Ident: CCB
Analysis from: 6/1/2021 10:17:47 AM
File: _2021-06-01_

Last save: 6/1/2021 10:44:18 AM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27149

Last save: 5/27/2021 12:48

SAMPLE:
: AM/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

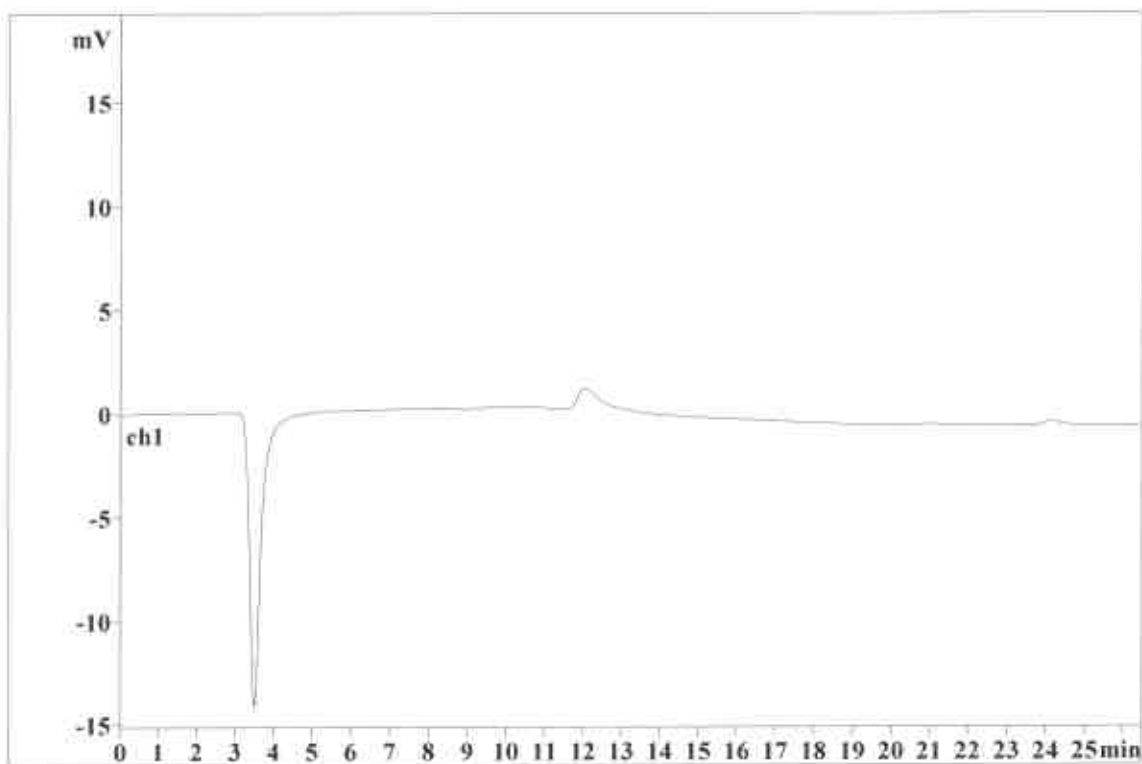

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 6/1/2021 4:33:33 PM
Printed by: wet


Ident: LB114681BLW
Analysis from: 6/1/2021 10:47:00 AM
File: _2021-06-01_

Last save: 6/1/2021 4:33:08 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27150

Last save: 5/27/2021 12:48

SAMPLE:
:
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

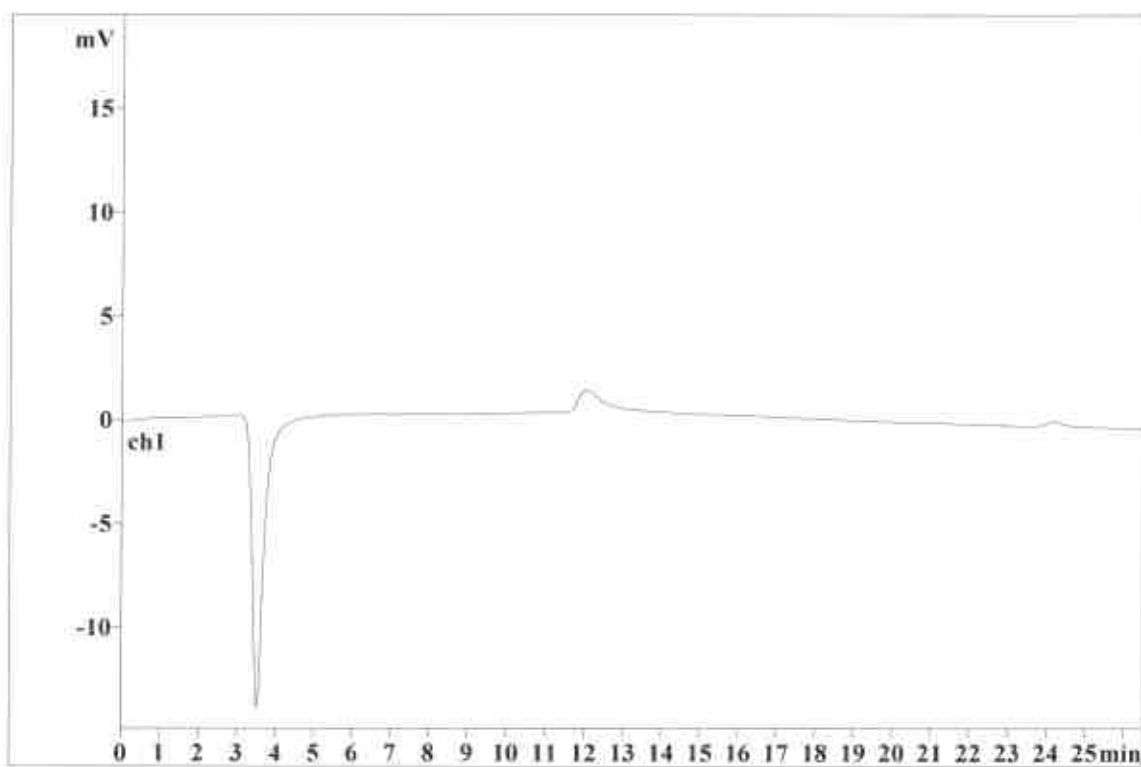

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 6/1/2021 4:33:40 PM
Printed by: wet


Ident: LB114681BSW
Analysis from: 6/1/2021 11:16:09 AM
File: 2021-06-01

Last save: 6/1/2021 4:33:08 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27151

Last save: 5/27/2021 12:48

SAMPLE:
: AM/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

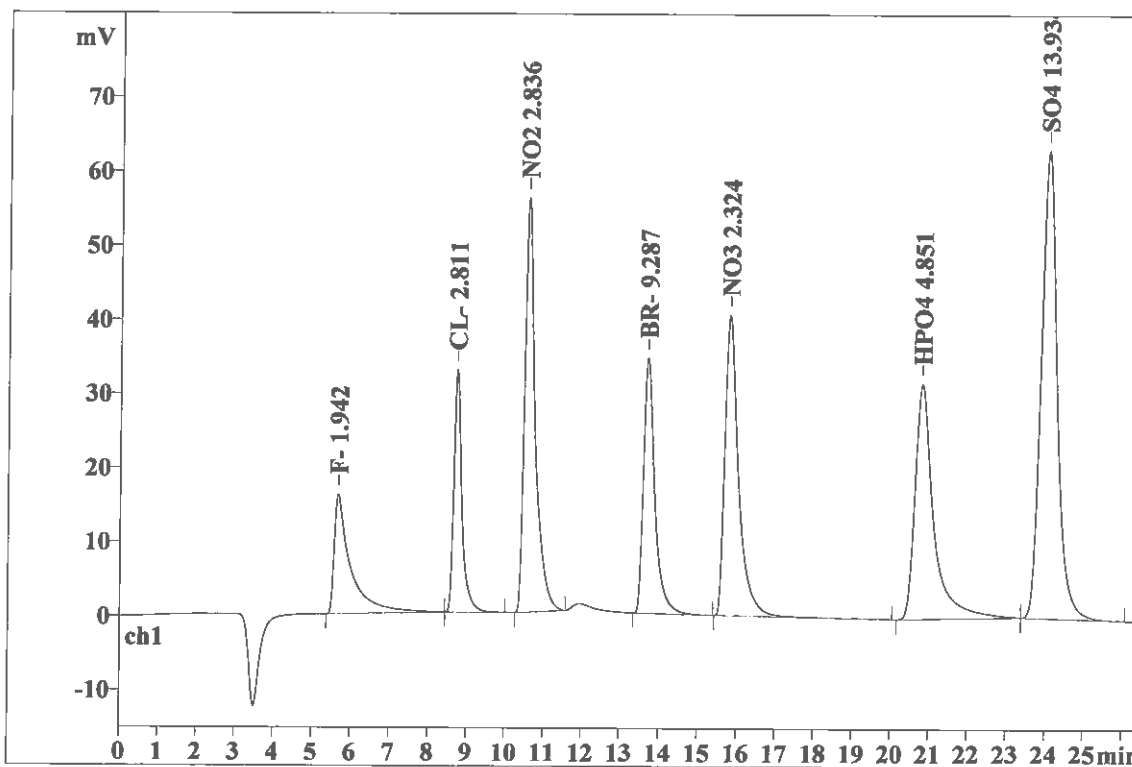

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.67	0.347	16.09	5.86	471.182	7.12
2	8.72	0.202	32.72	11.92	474.239	7.17
3	10.57	0.262	55.88	20.36	1068.676	16.15
4	13.69	0.291	34.44	12.55	699.817	10.57
5	15.78	0.350	40.51	14.76	996.633	15.06
6	20.79	0.449	31.72	11.56	1073.782	16.22
7	24.04	0.431	63.07	22.98	1833.994	27.71
7	26.50	0.333	274.43	100.00	6618.323	100.00

This report has been created by IC Net
METROHM LTD

Report date: 6/1/2021 4:33:47 PM
Printed by: wet


Ident: M2262-07
Analysis from: 6/1/2021 11:45:17 AM
File: _2021-06-01_

Last save: 6/1/2021 12:11:47 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27152

Last save: 5/27/2021 12:48

SAMPLE:
: AM/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

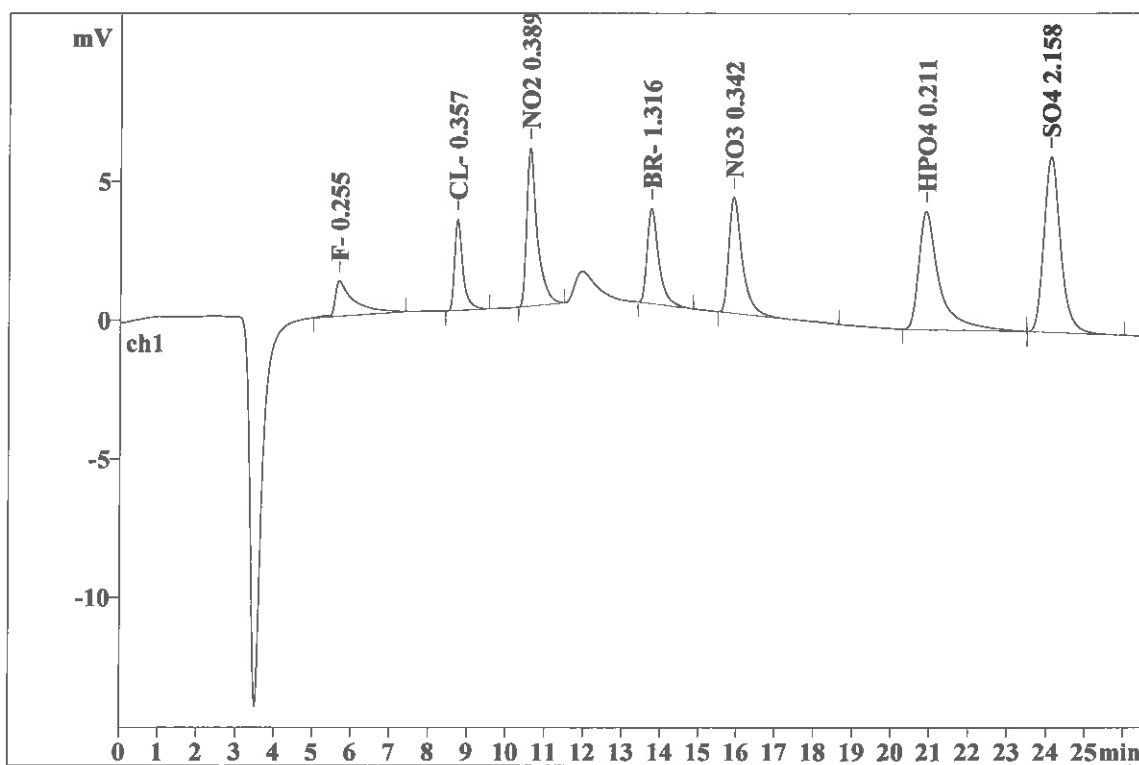

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.67	0.404	1.26	4.45	43.099	5.97
2	8.72	0.208	3.28	11.53	48.439	6.71
3	10.59	0.264	5.69	20.02	107.948	14.96
4	13.73	0.304	3.42	12.01	71.759	9.94
5	15.88	0.353	4.18	14.69	102.862	14.25
6	20.86	0.482	4.26	14.99	157.381	21.80
7	24.08	0.447	6.34	22.28	190.296	26.36
7	26.50	0.352	28.44	99.98	721.784	100.00

This report has been created by IC Net
METROHM LTD

Report date: 6/1/2021 4:33:55 PM
Printed by: wet


Ident: M2262-08
Analysis from: 6/1/2021 12:43:35 PM
File: _2021-06-01_

Last save: 6/1/2021 1:10:05 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27154

Last save: 5/27/2021 12:48

SAMPLE:
: AM/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

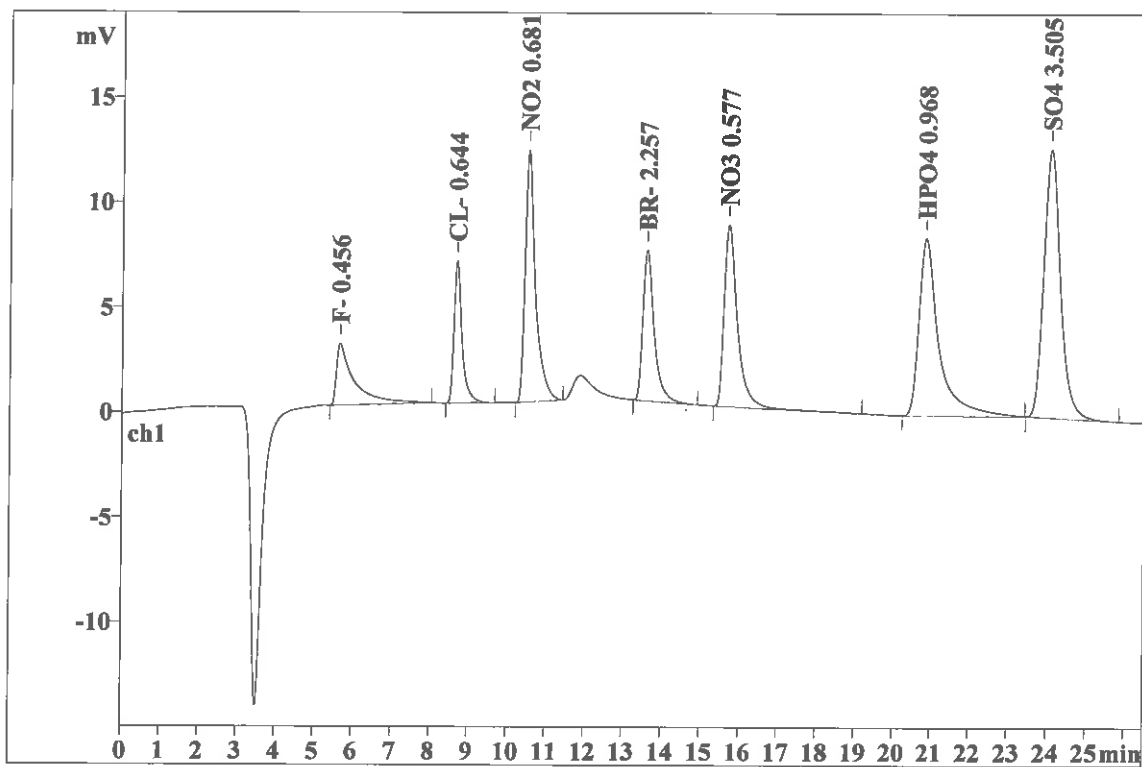

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.368	2.93	4.99	93.933	6.46
2	8.68	0.204	6.76	11.51	98.215	6.75
3	10.51	0.255	11.99	20.41	222.318	15.29
4	13.59	0.294	7.17	12.20	145.884	10.03
5	15.69	0.343	8.66	14.73	208.863	14.36
6	20.83	0.474	8.45	14.38	306.901	21.10
7	24.05	0.441	12.79	21.76	378.282	26.01
7	26.50	0.340	58.74	99.99	1454.396	100.00

This report has been created by IC Net
METROHM LTD

Report date: 6/1/2021 4:34:02 PM
Printed by: wet


Ident: CCV
Analysis from: 6/1/2021 1:17:17 PM
File: _2021-06-01_

Last save: 6/1/2021 1:43:47 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27155

Last save: 5/27/2021 12:48

SAMPLE:
: AM/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

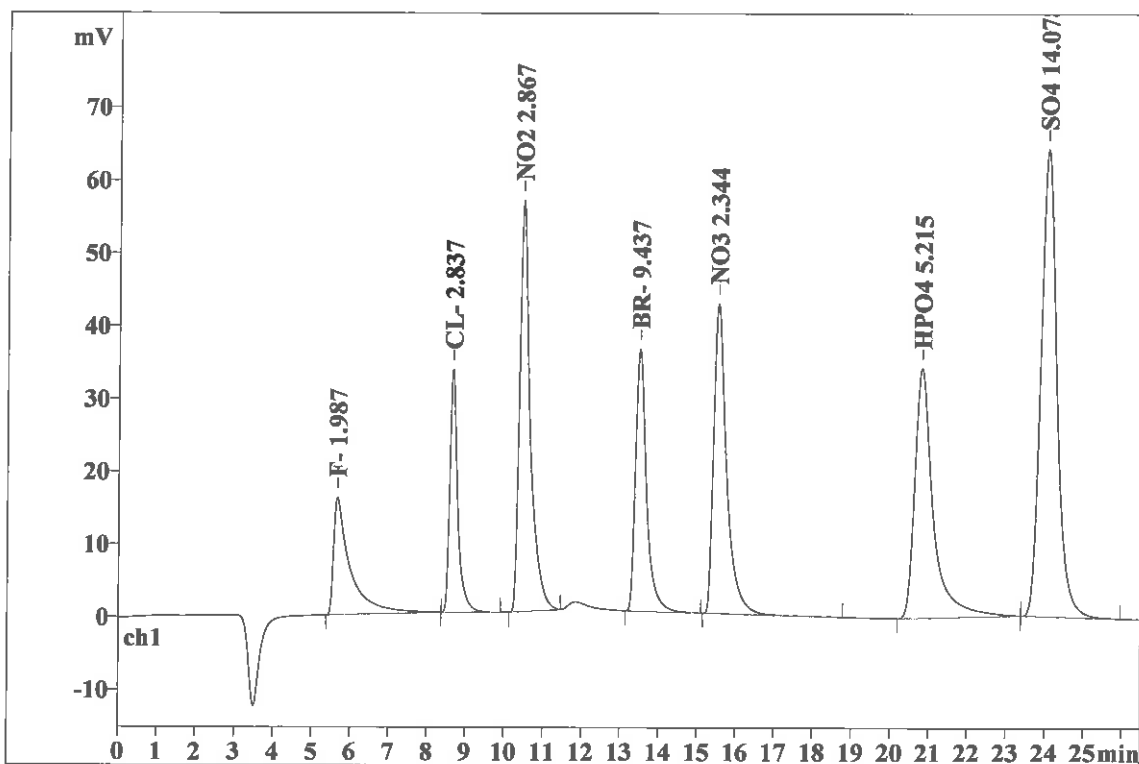

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.359	16.13	5.69	482.746	7.14
2	8.66	0.201	33.43	11.80	478.717	7.08
3	10.46	0.264	56.54	19.96	1080.986	15.99
4	13.49	0.283	36.05	12.72	711.578	10.53
5	15.52	0.338	42.58	15.03	1005.909	14.88
6	20.78	0.444	34.34	12.12	1145.790	16.95
7	24.04	0.430	64.21	22.67	1854.190	27.43
7	26.50	0.331	283.29	100.00	6759.916	100.00

This report has been created by IC Net
METROHM LTD

Report date: 6/1/2021 4:34:11 PM
Printed by: wet

Ident: CCB
Analysis from: 6/1/2021 2:01:17 PM
File: _2021-06-01_


Last save: 6/1/2021 2:27:47 PM

Method: AnionsIC2-052421.mtw
Run operator: wet
Analysis number: 27156

Last save: 5/27/2021 12:48

SAMPLE:

: AM/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

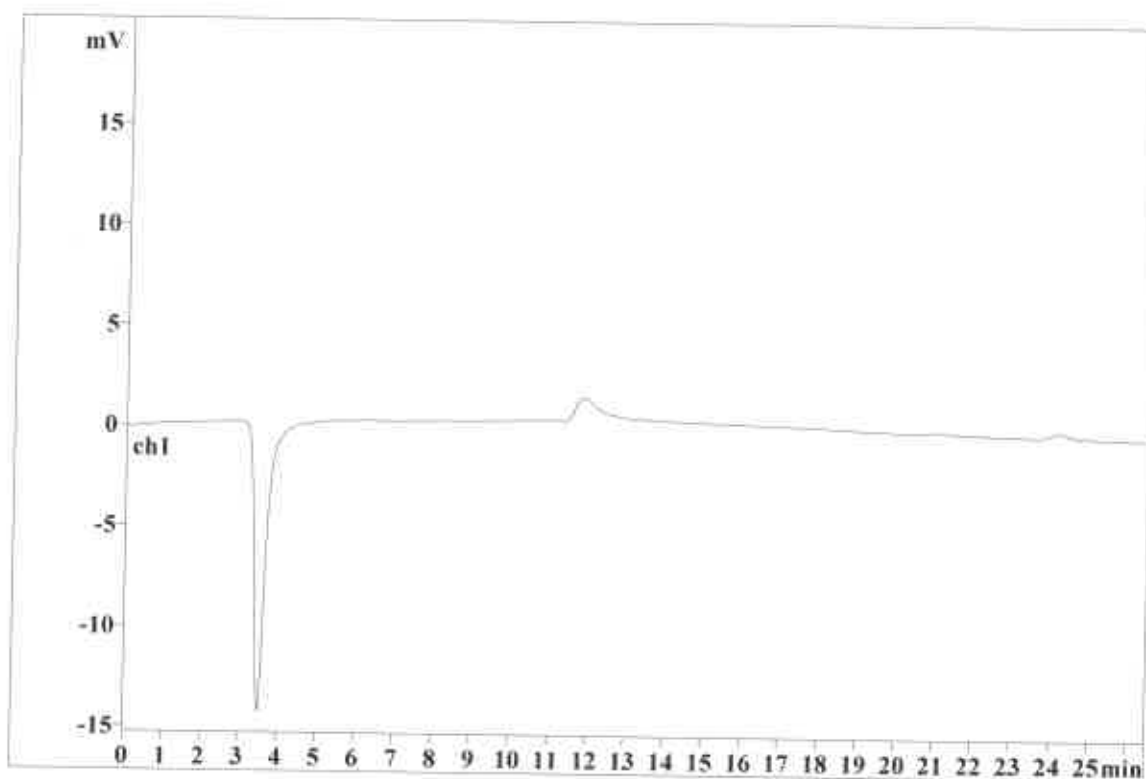

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD