


LB114742

7470A

INSTRUMENT ID: CV1

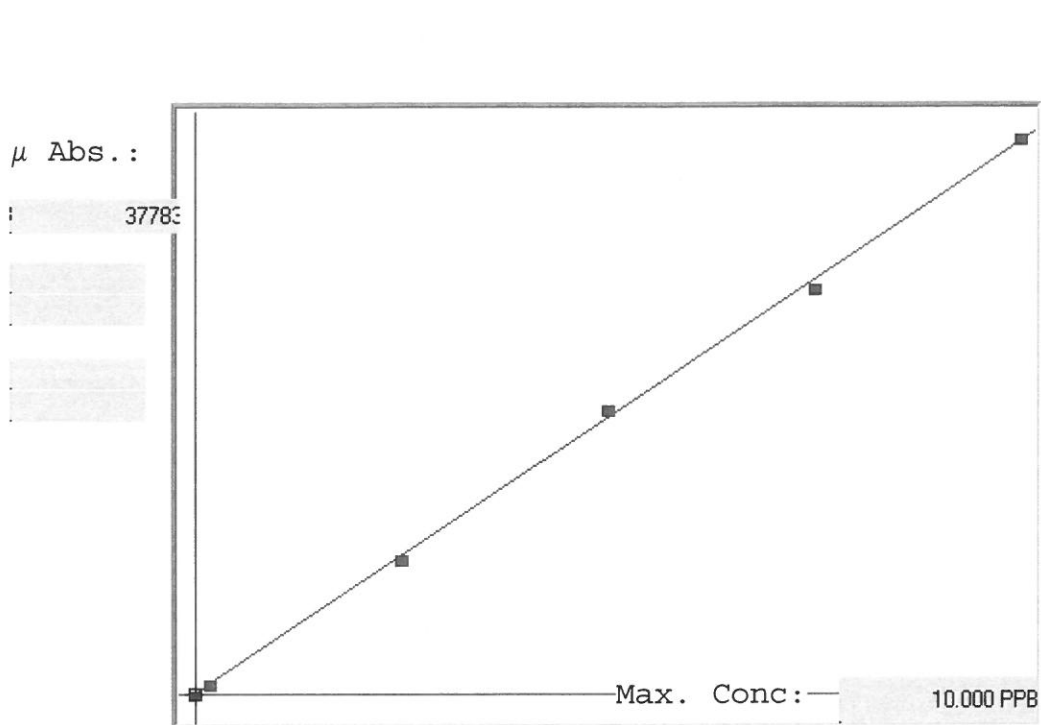

Linear

A= 0.0000e+000

B= 2.6569e-004

C= -1.6416e-003

Rho= 0.9997262

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.005	0.005	24	0.000	24					-
0.2	0.200	0.197	-0.003	746	0.0 %	746					-2
2.5	2.500	2.451	-0.049	9232	0.0 %	9232					-2
5.0	5.000	5.148	0.148	19383	0.0 %	19383					3
7.5	7.500	7.362	-0.138	27716	0.0 %	27716					-2
10.0	10.000	10.037	0.037	37783	0.0 %	37783					0

LB114742 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Jun 2021 15:08:55

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	24	-	0.0000	7470A	PPB	02 Jun 2021 15:11:03	S	Std
0.2 - 1	502	746	-	0.2000	7470A	PPB	02 Jun 2021 15:13:20	S	Std
2.5 - 1	525	9232	-	2.5000	7470A	PPB	02 Jun 2021 15:15:37	S	Std
5.0 - 1	55	19383	-	5.0000	7470A	PPB	02 Jun 2021 15:17:53	S	Std
7.5 - 1	57.5	27716	-	7.5000	7470A	PPB	02 Jun 2021 15:20:09	S	Std
10.0 - 1	510	37783	-	10.0000	7470A	PPB	02 Jun 2021 15:22:25	S	Std
ICV45 - 1	ICV45	14276	3.7914	-	7470A	PPB	02 Jun 2021 15:25:11	U	SMPL
ICB45 - 1	ICB45	-77	-0.0221	-	7470A	PPB	02 Jun 2021 15:27:26	U	SMPL
CCV04 - 1	CCV04	18775	4.9867	-	7470A	PPB	02 Jun 2021 15:29:40	U	SMPL
CCB04 - 1	CCB04	-98	-0.0277	-	7470A	PPB	02 Jun 2021 15:31:56	U	SMPL
CRA - 1	CRA	732	0.1928	-	7470A	PPB	02 Jun 2021 15:34:12	U	SMPL
HighStd - 1	HighStd	37274	9.9017	-	7470A	PPB	02 Jun 2021 15:36:26	U	SMPL
ChkStd - 1	ChkStd	26109	6.9353	-	7470A	PPB	02 Jun 2021 15:38:42	U	SMPL
PB136754BL - 1	PBW	-123	-0.0343	-	7470A	PPB	02 Jun 2021 15:40:58	U	SMPL
PB136754BS - 1	LCSW	14710	3.9067	-	7470A	PPB	02 Jun 2021 15:43:16	U	SMPL
M2569-05 - 1	MC0AA1	-62	-0.0181	-	7470A	PPB	02 Jun 2021 15:45:32	U	SMPL
M2569-05DUP - 1	MC0AA1DUP	5	-0.0003	-	7470A	PPB	02 Jun 2021 15:47:48	U	SMPL
M2569-05MS - 1	MC0AA1MS	14194	3.7696	-	7470A	PPB	02 Jun 2021 15:50:05	U	SMPL
M2569-05MSD - 1	MC0AA1MSD	14016	3.7223	-	7470A	PPB	02 Jun 2021 15:52:22	U	SMPL
PB136755BL - 1	PBW	-74	-0.0213	-	7470A	PPB	02 Jun 2021 15:54:37	U	SMPL
CCV05 - 1	CCV05	19123	5.0792	-	7470A	PPB	02 Jun 2021 15:56:52	U	SMPL
CCB05 - 1	CCB05	-91	-0.0258	-	7470A	PPB	02 Jun 2021 15:59:07	U	SMPL
PB136755BS - 1	LCSW	15094	4.0087	-	7470A	PPB	02 Jun 2021 16:01:22	U	SMPL
M2563-03 - 1	33213-14	-59	-0.0173	-	7470A	PPB	02 Jun 2021 16:03:38	U	SMPL
M2569-09 - 1	MC0AA0	30	0.0063	-	7470A	PPB	02 Jun 2021 16:05:54	U	SMPL
M2569-09DUP - 1	MC0AA0DUP	52	0.0122	-	7470A	PPB	02 Jun 2021 16:08:10	U	SMPL
M2569-09MS - 1	MC0AA0MS	15006	3.9853	-	7470A	PPB	02 Jun 2021 16:10:26	U	SMPL
M2569-09MSD - 1	MC0AA0MSD	14586	3.8737	-	7470A	PPB	02 Jun 2021 16:12:42	U	SMPL
CCV06 - 1	CCV06	19648	5.2187	-	7470A	PPB	02 Jun 2021 16:14:59	U	SMPL
CCB06 - 1	CCB06	-65	-0.0189	-	7470A	PPB	02 Jun 2021 16:17:15	U	SMPL
PB136754TB - 1	PB136727TB	14	0.0021	-	7470A	PPB	02 Jun 2021 16:19:32	U	SMPL
PB136755TB - 1	PB136730TB	25	0.0050	-	7470A	PPB	02 Jun 2021 16:21:48	U	SMPL
M2569-05LX5 - 1		24	0.0047	-	7470A	PPB	02 Jun 2021 16:24:03	U	SMPL
M2569-05A - 1		14958	3.9726	-	7470A	PPB	02 Jun 2021 16:26:22	U	SMPL
M2569-09LX5 - 1		-52	-0.0155	-	7470A	PPB	02 Jun 2021 16:28:37	U	SMPL
M2569-09A - 1		15443	4.1014	-	7470A	PPB	02 Jun 2021 16:30:53	U	SMPL
CCV07 - 1	CCV07	19419	5.1578	-	7470A	PPB	02 Jun 2021 16:33:08	U	SMPL
CCB07 - 1	CCB07	-68	-0.0197	-	7470A	PPB	02 Jun 2021 16:35:24	U	SMPL