


LB114775

7471B

INSTRUMENT ID: CV1

Linear

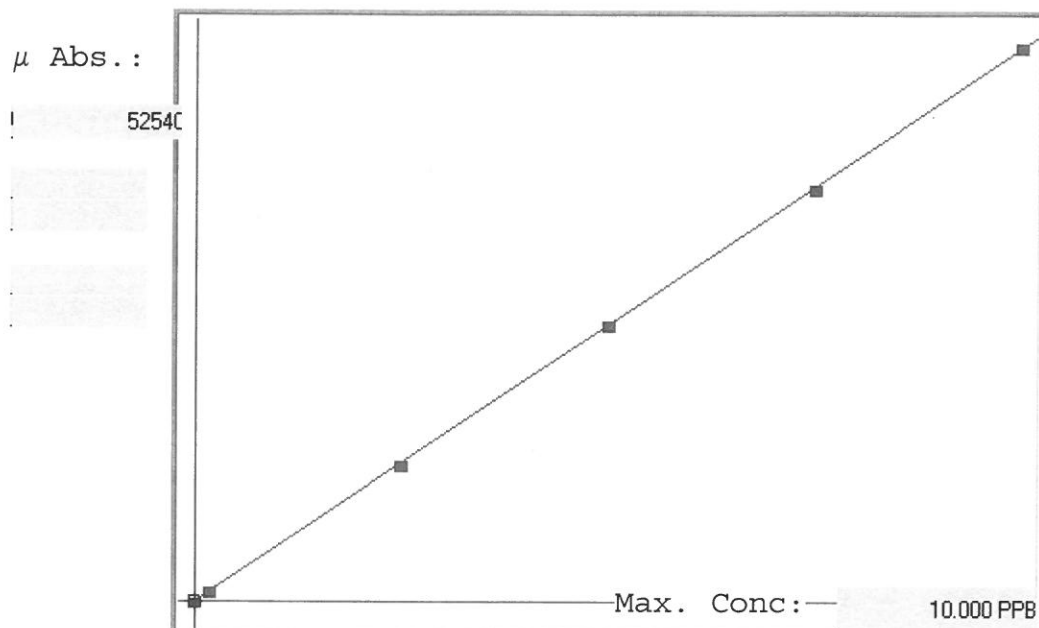

A= 0.0000e+000

B= 1.9065e-004

C= 3.7761e-003

Rho= 0.9999875

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.010	0.010	35	0.000	35				
0.2	0.200	0.207	0.007	1067	0.0 %	1067				
2.5	2.500	2.478	-0.022	12979	0.0 %	12979				
5.0	5.000	5.013	0.013	26272	0.0 %	26272				
7.5	7.500	7.471	-0.029	39168	0.0 %	39168				
10.0	10.000	10.020	0.020	52540	0.0 %	52540				

0.000
131000

LB114775 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 04 Jun 2021 13:27:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	35	-	0.0000	7471B	PPB	04 Jun 2021 13:35:21	S	Std
0.2 - 1	50.2	1067	-	0.2000	7471B	PPB	04 Jun 2021 13:37:38	S	Std
2.5 - 1	52.5	12979	-	2.5000	7471B	PPB	04 Jun 2021 13:39:55	S	Std
5.0 - 1	55	26272	-	5.0000	7471B	PPB	04 Jun 2021 13:42:12	S	Std
7.5 - 1	57.5	39168	-	7.5000	7471B	PPB	04 Jun 2021 13:47:04	S	Std
10.0 - 1	59.5	52540	-	10.0000	7471B	PPB	04 Jun 2021 13:49:19	S	Std
ICV48 - 1	ICV48	20815	3.9721	-	7471B	PPB	04 Jun 2021 13:52:02	U	SMPL
ICB48 - 1	ICB48	-85	-0.0124	-	7471B	PPB	04 Jun 2021 13:54:16	U	SMPL
CCV19 - 1	CCV19	27488	5.2443	-	7471B	PPB	04 Jun 2021 13:56:32	U	SMPL
CCB19 - 1	CCB19	-101	-0.0155	-	7471B	PPB	04 Jun 2021 13:58:47	U	SMPL
CRA - 1	CRA	1033	0.2007	-	7471B	PPB	04 Jun 2021 14:01:02	U	SMPL
HighStd - 1	HighStd	51711	9.8624	-	7471B	PPB	04 Jun 2021 14:03:17	U	SMPL
ChkStd - 1	ChkStd	36600	6.9815	-	7471B	PPB	04 Jun 2021 14:05:33	U	SMPL
PB136818BL - 1	PB136818BL	-151	-0.0250	-	7471B	PPB	04 Jun 2021 14:07:49	U	SMPL
PB136818BS - 1	PB136818BS	19631	3.7464	-	7471B	PPB	04 Jun 2021 14:10:06	U	SMPL
M2589-01 - 1	18-B7(0-2)	19367	3.6961	-	7471B	PPB	04 Jun 2021 14:12:22	U	SMPL
M2589-02 - 1	18-B7(2-4)	14054	2.6832	-	7471B	PPB	04 Jun 2021 14:14:38	U	SMPL
M2589-03 - 1	18-B7(4-6)	14666	2.7998	-	7471B	PPB	04 Jun 2021 14:16:56	U	SMPL
M2589-04 - 1	18-B8(0-2)	16485	3.1466	-	7471B	PPB	04 Jun 2021 14:19:13	U	SMPL
M2589-05 - 1	18-B8(2-4)	6914	1.3219	-	7471B	PPB	04 Jun 2021 14:21:28	U	SMPL
CCV20 - 1	CCV20	27237	5.1965	-	7471B	PPB	04 Jun 2021 14:23:43	U	SMPL
CCB20 - 1	CCB20	-77	-0.0109	-	7471B	PPB	04 Jun 2021 14:25:58	U	SMPL
M2589-06 - 1	18-B8(4-6)	11070	2.1143	-	7471B	PPB	04 Jun 2021 14:28:13	U	SMPL
M2589-07 - 1	18-B9(0-2)	3382	0.6486	-	7471B	PPB	04 Jun 2021 14:30:28	U	SMPL
M2589-08 - 1	18-B9(2-4)	4416	0.8457	-	7471B	PPB	04 Jun 2021 14:32:44	U	SMPL
M2589-09 - 1	18-B9(4-6)	8465	1.6176	-	7471B	PPB	04 Jun 2021 14:34:59	U	SMPL
M2589-10 - 1	FOUNDATION-EXCAVATION-SAMPLE-A	7306	1.3967	-	7471B	PPB	04 Jun 2021 14:37:15	U	SMPL
M2589-11 - 1	18-B10(0-2)	7287	1.3930	-	7471B	PPB	04 Jun 2021 14:39:32	U	SMPL
M2589-12 - 1	18-B10(2-4)	16833	3.2130	-	7471B	PPB	04 Jun 2021 14:41:48	U	SMPL
M2589-13 - 1	18-B10(4-6)	27303	5.2091	-	7471B	PPB	04 Jun 2021 14:44:06	U	SMPL
M2589-14 - 1	18-B11(0-2)	19212	3.6665	-	7471B	PPB	04 Jun 2021 14:46:24	U	SMPL
M2589-15 - 1	18-B11(2-4)	64553	12.3108	-	7471B	PPB	04 Jun 2021 14:48:40	U	SMPL
CCV21 - 1	CCV21	27275	5.2037	-	7471B	PPB	04 Jun 2021 14:50:55	U	SMPL
CCB21 - 1	CCB21	-122	-0.0195	-	7471B	PPB	04 Jun 2021 14:53:12	U	SMPL
M2589-16 - 1	18-B11(4-6)	6224	1.1904	-	7471B	PPB	04 Jun 2021 14:55:28	U	SMPL
M2589-17 - 1	FOUNDATION-EXCAVATION-SAMPLE-B	43778	8.3500	-	7471B	PPB	04 Jun 2021 14:57:44	U	SMPL
M2589-18 - 1	18-B12(0-2)	6819	1.3038	-	7471B	PPB	04 Jun 2021 14:59:59	U	SMPL
M2589-19 - 1	18-B12(2-4)	7429	1.4201	-	7471B	PPB	04 Jun 2021 15:02:15	U	SMPL
M2589-20 - 1	18-B12(4-6)	28608	5.4579	-	7471B	PPB	04 Jun 2021 15:04:31	U	SMPL
M2589-20DUP - 1	18-B12(4-6)DUP	25518	4.8688	-	7471B	PPB	04 Jun 2021 15:06:47	U	SMPL
M2589-20MS - 1	18-B12(4-6)MS	46902	8.9456	-	7471B	PPB	04 Jun 2021 15:09:04	U	SMPL
M2589-20MSD - 1	18-B12(4-6)MSD	48297	9.2116	-	7471B	PPB	04 Jun 2021 15:14:13	U	SMPL
PB136819BL - 1	PB136819BL	-84	-0.0122	-	7471B	PPB	04 Jun 2021 15:16:30	U	SMPL
PB136819BS - 1	PB136819BS	18583	3.5466	-	7471B	PPB	04 Jun 2021 15:18:47	U	SMPL
CCV22 - 1	CCV22	26069	4.9738	-	7471B	PPB	04 Jun 2021 15:21:02	U	SMPL
CCB22 - 1	CCB22	-32	-0.0023	-	7471B	PPB	04 Jun 2021 15:23:18	U	SMPL
M2597-01 - 1	124019	1223	0.2369	-	7471B	PPB	04 Jun 2021 15:25:34	U	SMPL
M2597-03 - 1	124042	3109	0.5965	-	7471B	PPB	04 Jun 2021 15:27:49	U	SMPL
M2598-01 - 1	23	766	0.1498	-	7471B	PPB	04 Jun 2021 15:30:05	U	SMPL
M2598-04 - 1	19	6989	1.3362	-	7471B	PPB	04 Jun 2021 15:32:19	U	SMPL
M2598-07 - 1	13	3450	0.6615	-	7471B	PPB	04 Jun 2021 15:34:35	U	SMPL
M2598-10 - 1	17	6158	1.1778	-	7471B	PPB	04 Jun 2021 15:36:51	U	SMPL
M2599-01 - 1	339	29409	5.6106	-	7471B	PPB	04 Jun 2021 15:39:07	U	SMPL
M2601-01 - 1	VNJ-236	2037	0.3921	-	7471B	PPB	04 Jun 2021 15:41:24	U	SMPL
M2601-05 - 1	RO-CHRT-27166	3274	0.6280	-	7471B	PPB	04 Jun 2021 15:43:41	U	SMPL
M2602-01 - 1	SU-02-060321	1338	0.2589	-	7471B	PPB	04 Jun 2021 15:45:56	U	SMPL
CCV23 - 1	CCV23	25918	4.9450	-	7471B	PPB	04 Jun 2021 15:48:12	U	SMPL
CCB23 - 1	CCB23	-33	-0.0025	-	7471B	PPB	04 Jun 2021 15:50:27	U	SMPL
M2611-01 - 1	T-1	2945	0.5652	-	7471B	PPB	04 Jun 2021 15:52:42	U	SMPL
M2611-01DUP - 1	T-1DUP	2978	0.5715	-	7471B	PPB	04 Jun 2021 15:57:43	U	SMPL
M2611-01MS - 1	T-1MS	22511	4.2955	-	7471B	PPB	04 Jun 2021 15:59:58	U	SMPL
M2611-01MSD - 1	T-1MSD	23777	4.5368	-	7471B	PPB	04 Jun 2021 16:02:14	U	SMPL
M2589-20LX5 - 1		5413	1.0358	-	7471B	PPB	04 Jun 2021 16:04:30	U	SMPL
M2589-20A - 1		46333	8.8371	-	7471B	PPB	04 Jun 2021 16:06:46	U	SMPL
M2611-01LX5 - 1		402	0.0804	-	7471B	PPB	04 Jun 2021 16:09:02	U	SMPL
M2611-01A - 1		23682	4.5187	-	7471B	PPB	04 Jun 2021 16:11:19	U	SMPL
CCV24 - 1	CCV24	25778	4.9183	-	7471B	PPB	04 Jun 2021 16:13:36	U	SMPL
CCB24 - 1	CCB24	-69	-0.0094	-	7471B	PPB	04 Jun 2021 16:15:52	U	SMPL
M2583-01 - 1	39-41S	6294	1.2037	-	7471B	PPB	04 Jun 2021 16:18:08	U	SMPL
M2583-02 - 1	54-57S	10011	1.9124	-	7471B	PPB	04 Jun 2021 16:20:25	U	SMPL
M2589-15DLX2 - 1		30519	5.8222	-	7471B	PPB	04 Jun 2021 16:22:41	U	SMPL
CCV25 - 1	CCV25	27081	5.1668	-	7471B	PPB	04 Jun 2021 16:24:59	U	SMPL
CCB25 - 1	CCB25	-73	-0.0101	-	7471B	PPB	04 Jun 2021 16:27:15	U	SMPL