


LB114906

SFAM01.1

INSTRUMENT ID: CV2

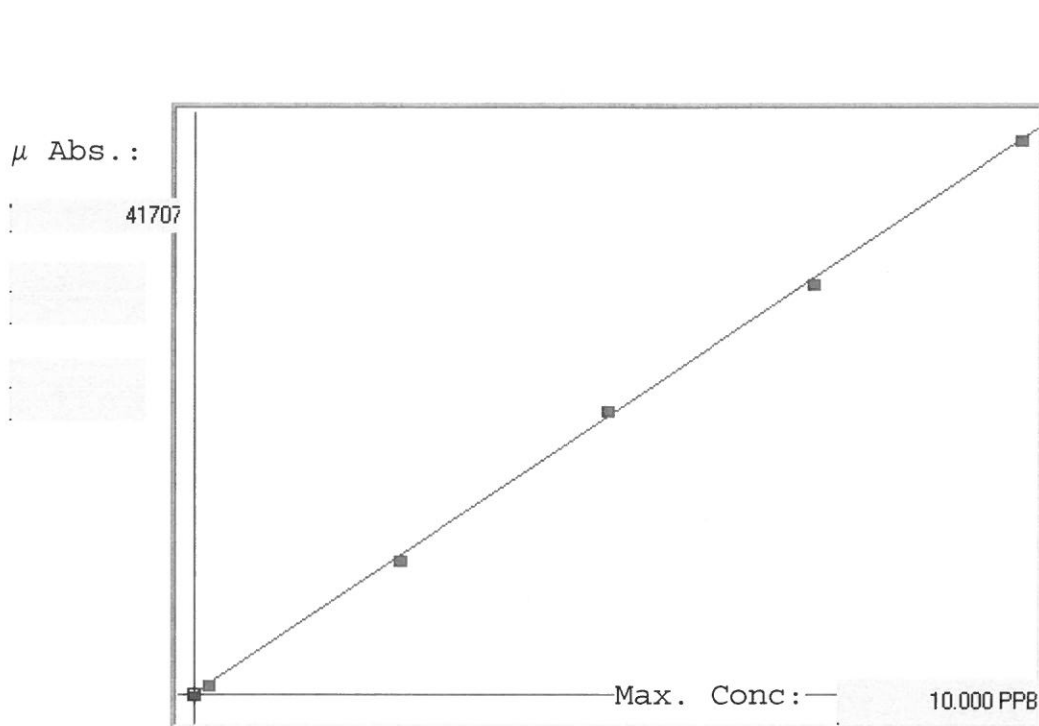

A= 0.0000e+000

B= 2.3976e-004 slope

C= -1.1334e-003 y-intercept

Rho= 0.9998444

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.008	0.008	37	0.000	37					
0.05	0.050					204					
0.20	0.200	0.201	0.001	842	0.0 %	842					
2.50	2.500	2.428	-0.072	10131	0.0 %	10131					
5.00	5.000	5.128	0.128	21391	0.0 %	21391					
7.50	7.500	7.438	-0.062	31026	0.0 %	31026					
10.0	10.000	9.998	-0.002	41707	0.0 %	41707					

11-33-10

LB114906
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	37	-		0 SFAM01.1	PPB	6/11/2021 13:42	Std
	0.2 S01	842	-		0.2 SFAM01.1	PPB	6/11/2021 13:44	Std
	2.5 S02	10131	-		2.5 SFAM01.1	PPB	6/11/2021 13:47	Std
	5 S03	21391	-		5 SFAM01.1	PPB	6/11/2021 13:49	Std
	7.5 S04	31026	-		7.5 SFAM01.1	PPB	6/11/2021 13:51	Std
	10 S05	41707	-		10 SFAM01.1	PPB	6/11/2021 13:53	Std
ICV039	ICV039	16840	4.0364 -		SFAM01.1	PPB	6/11/2021 13:56	SMPL
ICB039	ICB039	-164	-0.0405 -		SFAM01.1	PPB	6/11/2021 13:58	SMPL
CCV079	CCV079	20865	5.0014 -		SFAM01.1	PPB	6/11/2021 14:01	SMPL
CCB079	CCB079	-172	-0.0424 -		SFAM01.1	PPB	6/11/2021 14:03	SMPL
PB137025BL	PBW025	-33	-0.009 -		SFAM01.1	PPB	6/11/2021 14:05	SMPL
M2557-07	X3489	20451	4.9022 -		SFAM01.1	PPB	6/11/2021 14:10	SMPL
M2557-08	X3489D	20320	4.8708 -		SFAM01.1	PPB	6/11/2021 14:14	SMPL
M2557-09	X3489S	24632	5.9046 -		SFAM01.1	PPB	6/11/2021 14:21	SMPL
CCV080	CCV080	20248	4.8535 -		SFAM01.1	PPB	6/11/2021 14:23	SMPL
CCB080	CCB080	-195	-0.0479 -		SFAM01.1	PPB	6/11/2021 14:26	SMPL