


LB114916

SFAM01.1

INSTRUMENT ID: CV1

 μ Abs.:

44113

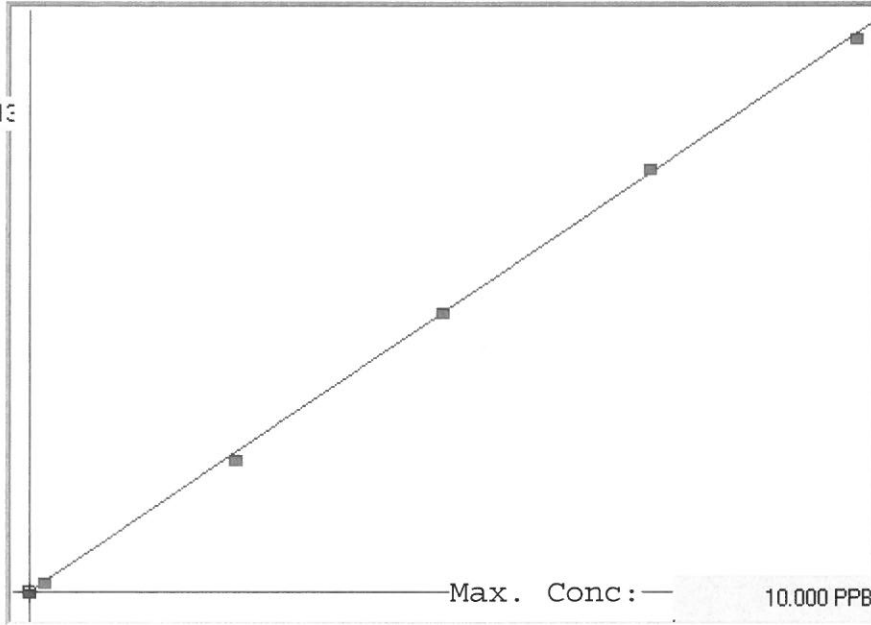

Linear

A= 0.0000e+000

B= 2.2471e-004 *slope*C= 1.3970e-002 *y-intercept*

Rho= 0.9998357

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	<i>01011</i>
0.00	0.000	0.018	0.018	16	0.000	16					<i>=</i>
0.05	0.050					204					<i>7</i>
0.20	0.200	0.213	0.013	884	0.0 %	884					<i>-4</i>
2.50	2.500	2.402	-0.098	10626	0.0 %	10626					<i>1</i>
5.00	5.000	5.044	0.044	22386	0.0 %	22386					<i>1</i>
7.50	7.500	7.597	0.097	33745	0.0 %	33745					<i>1</i>
10.0	10.000	9.927	-0.073	44113	0.0 %	44113					<i>1</i>

LB114916
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	16	-		0 SFAM01.1	PPB	6/11/2021 15:28	Std
	0.2 S01	884	-		0.2 SFAM01.1	PPB	6/11/2021 15:30	Std
	2.5 S02	10626	-		2.5 SFAM01.1	PPB	6/11/2021 15:35	Std
	5 S03	22386	-		5 SFAM01.1	PPB	6/11/2021 15:38	Std
	7.5 S04	33745	-		7.5 SFAM01.1	PPB	6/11/2021 15:40	Std
	10 S05	44113	-		10 SFAM01.1	PPB	6/11/2021 15:42	Std
ICV040	ICV040	17147	3.8671 -		SFAM01.1	PPB	6/11/2021 15:45	SMPL
ICB040	ICB040	-167	-0.0236 -		SFAM01.1	PPB	6/11/2021 15:47	SMPL
CCV081	CCV081	22210	5.0048 -		SFAM01.1	PPB	6/11/2021 15:49	SMPL
CCB081	CCB081	-166	-0.0233 -		SFAM01.1	PPB	6/11/2021 15:52	SMPL
PB137026BL	PBS026	-16	0.0104 -		SFAM01.1	PPB	6/11/2021 15:54	SMPL
M2557-19	X3493	18868	4.2539 -		SFAM01.1	PPB	6/11/2021 15:56	SMPL
M2557-20	X3493D	18132	4.0885 -		SFAM01.1	PPB	6/11/2021 16:01	SMPL
M2557-21	X3493S	28738	6.4718 -		SFAM01.1	PPB	6/11/2021 16:05	SMPL
CCV082	CCV082	21670	4.8835 -		SFAM01.1	PPB	6/11/2021 16:10	SMPL
CCB082	CCB082	-151	-0.02 -		SFAM01.1	PPB	6/11/2021 16:12	SMPL