


LB114939

7470A

INSTRUMENT ID: CV2

Linear

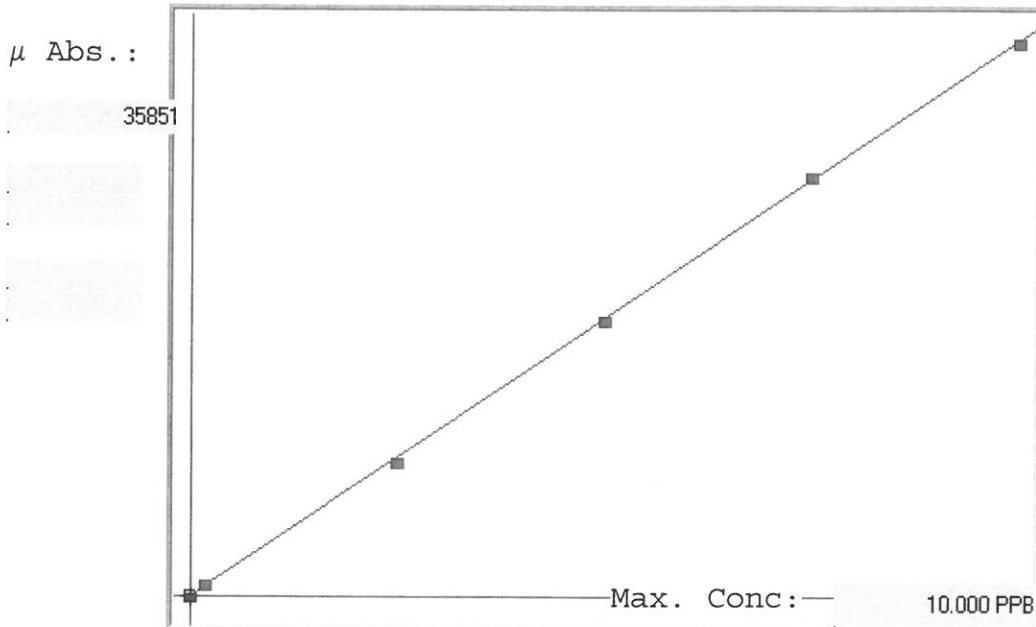

A= 0.0000e+000

B= 2.7784e-004

C= 8.1504e-004

Rho= 0.9999295

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.021	0.021	74	0.000	74					1
0.2	0.200	0.212	0.012	759	0.0 %	759					6
2.5	2.500	2.435	-0.065	8762	0.0 %	8762					3
5.0	5.000	4.997	-0.003	17984	0.0 %	17984					0
7.5	7.500	7.573	0.073	27252	0.0 %	27252					0
10.0	10.000	9.962	-0.038	35851	0.0 %	35851					0

LB114939 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Jun 2021 11:59:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	30	74	-	0.0000	7470A	PPB	13 Jun 2021 12:02:21	S	Std
0.2 - 1	50.2	759	-	0.2000	7470A	PPB	13 Jun 2021 12:04:38	S	Std
2.5 - 1	52.5	8762	-	2.5000	7470A	PPB	13 Jun 2021 12:06:55	S	Std
5.0 - 1	55	17984	-	5.0000	7470A	PPB	13 Jun 2021 12:09:12	S	Std
7.5 - 1	57.5	27252	-	7.5000	7470A	PPB	13 Jun 2021 12:14:02	S	Std
10.0 - 1	58	35851	-	10.0000	7470A	PPB	13 Jun 2021 12:18:54	S	Std
ICV60 - 1	ICV60	14423	4.0081	-	7470A	PPB	13 Jun 2021 12:21:34	U	SMPL
ICB60 - 1	ICB60	-149	-0.0406	-	7470A	PPB	13 Jun 2021 12:23:49	U	SMPL
CCV87 - 1	CCV87	17481	4.8577	-	7470A	PPB	13 Jun 2021 12:26:04	U	SMPL
CCB87 - 1	CCB87	-114	-0.0309	-	7470A	PPB	13 Jun 2021 12:28:19	U	SMPL
CRA - 1	CRA	689	0.1922	-	7470A	PPB	13 Jun 2021 12:30:34	U	SMPL
HighStd - 1	HighStd	35381	9.8311	-	7470A	PPB	13 Jun 2021 12:32:49	U	SMPL
ChkStd - 1	ChkStd	25788	7.1658	-	7470A	PPB	13 Jun 2021 12:35:04	U	SMPL
PB136994BL - 1	PBW	-2	0.0003	-	7470A	PPB	13 Jun 2021 12:40:03	U	SMPL
PB136994BS - 1	LCSW	14416	4.0062	-	7470A	PPB	13 Jun 2021 12:42:18	U	SMPL
M2638-04 - 1	ND-1	-78	-0.0209	-	7470A	PPB	13 Jun 2021 12:44:34	U	SMPL
M2638-04DUP - 1	ND-1DUP	8	0.0030	-	7470A	PPB	13 Jun 2021 12:46:51	U	SMPL
M2638-04MS - 1	ND-1MS	15128	4.2040	-	7470A	PPB	13 Jun 2021 12:49:07	U	SMPL
M2638-04MSD - 1	ND-1MSD	14281	3.9687	-	7470A	PPB	13 Jun 2021 12:51:25	U	SMPL
M2644-01 - 1	1846-75-76	-121	-0.0328	-	7470A	PPB	13 Jun 2021 12:53:39	U	SMPL
CCV88 - 1	CCV88	17842	4.9580	-	7470A	PPB	13 Jun 2021 12:55:54	U	SMPL
CCB88 - 1	CCB88	-127	-0.0345	-	7470A	PPB	13 Jun 2021 12:58:09	U	SMPL
M2644-03 - 1	1894-1900	-11	-0.0022	-	7470A	PPB	13 Jun 2021 13:00:25	U	SMPL
M2658-02 - 1	T-FLOOR	28	0.0086	-	7470A	PPB	13 Jun 2021 13:02:40	U	SMPL
M2658-05 - 1	P-WALL	70	0.0203	-	7470A	PPB	13 Jun 2021 13:04:55	U	SMPL
M2658-08 - 1	G-FLOOR-1	53	0.0155	-	7470A	PPB	13 Jun 2021 13:07:11	U	SMPL
M2658-11 - 1	G-FLOOR-2	64	0.0186	-	7470A	PPB	13 Jun 2021 13:09:27	U	SMPL
M2658-14 - 1	G-WALL-1	80	0.0230	-	7470A	PPB	13 Jun 2021 13:11:42	U	SMPL
M2658-17 - 1	G-WALL-2	87	0.0250	-	7470A	PPB	13 Jun 2021 13:13:59	U	SMPL
M2659-01 - 1	31454	748	0.2086	-	7470A	PPB	13 Jun 2021 13:16:16	U	SMPL
PB137027BL - 1	PBW	-163	-0.0445	-	7470A	PPB	13 Jun 2021 13:18:33	U	SMPL
PB137027BS - 1	LCSW	12567	3.4924	-	7470A	PPB	13 Jun 2021 13:20:49	U	SMPL
CCV89 - 1	CCV89	16457	4.5732	-	7470A	PPB	13 Jun 2021 13:23:04	U	SMPL
CCB89 - 1	CCB89	-156	-0.0425	-	7470A	PPB	13 Jun 2021 13:25:20	U	SMPL
M2673-04 - 1	17-B6(88-92)	17	0.0055	-	7470A	PPB	13 Jun 2021 13:27:36	U	SMPL
M2673-04DUP - 1	17-B6(88-92)DUP	19	0.0061	-	7470A	PPB	13 Jun 2021 13:29:51	U	SMPL
M2673-04MS - 1	17-B6(88-92)MS	13378	3.7178	-	7470A	PPB	13 Jun 2021 13:40:40	U	SMPL
M2673-04MSD - 1	17-B6(88-92)MSD	14641	4.0687	-	7470A	PPB	13 Jun 2021 13:42:55	U	SMPL
M2673-05 - 1	17-B6(92-96)	-21	-0.0050	-	7470A	PPB	13 Jun 2021 13:45:11	U	SMPL
M2673-06 - 1	17-B6(96-100)	23	0.0072	-	7470A	PPB	13 Jun 2021 13:47:27	U	SMPL
M2674-07 - 1	TMR-DS-01-060921	-5	-0.0006	-	7470A	PPB	13 Jun 2021 13:49:43	U	SMPL
M2674-08 - 1	TMR-DS-02-060921	27	0.0083	-	7470A	PPB	13 Jun 2021 13:52:00	U	SMPL
M2674-09 - 1	TMR-DS-03-060921	28	0.0086	-	7470A	PPB	13 Jun 2021 13:54:17	U	SMPL
M2674-10 - 1	TMR-DS-04-060921	21	0.0066	-	7470A	PPB	13 Jun 2021 13:56:32	U	SMPL
CCV90 - 1	CCV90	18926	5.2592	-	7470A	PPB	13 Jun 2021 13:58:47	U	SMPL
CCB90 - 1	CCB90	-152	-0.0414	-	7470A	PPB	13 Jun 2021 14:01:03	U	SMPL
M2674-11 - 1	TMR-DS-05-060921	8	0.0030	-	7470A	PPB	13 Jun 2021 14:03:18	U	SMPL
M2674-12 - 1	TMR-DS-06-060921	111	0.0317	-	7470A	PPB	13 Jun 2021 14:05:34	U	SMPL
M2675-03 - 1	BS-RO-COMP	-51	-0.0134	-	7470A	PPB	13 Jun 2021 14:07:50	U	SMPL
PB136994TB - 1	PB136962TB	-7	-0.0011	-	7470A	PPB	13 Jun 2021 14:10:05	U	SMPL
PB137027TB - 1	PB136985TB	-8	-0.0014	-	7470A	PPB	13 Jun 2021 14:12:21	U	SMPL
M2638-04LX5 - 1		-7	-0.0011	-	7470A	PPB	13 Jun 2021 14:14:37	U	SMPL
M2638-04A - 1		15044	4.1806	-	7470A	PPB	13 Jun 2021 14:25:49	U	SMPL
M2673-04LX5 - 1		-131	-0.0356	-	7470A	PPB	13 Jun 2021 14:28:07	U	SMPL
M2673-04A - 1		14777	4.1065	-	7470A	PPB	13 Jun 2021 14:30:23	U	SMPL
CCV91 - 1	CCV91	18576	5.1620	-	7470A	PPB	13 Jun 2021 14:32:39	U	SMPL
CCB91 - 1	CCB91	-117	-0.0317	-	7470A	PPB	13 Jun 2021 14:34:54	U	SMPL