


Clear table

Instrument ID: IC-1										Analyst : AP		Method: 300.0	
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-06-08_	6/8/21 8:56		AP/MA		
STD2	0.4410	0.6970	0.7050	2.3390	0.6050	0.9350	3.4730	2021-06-08_	6/8/21 9:26		AP/MA		
STD3	0.7910	1.2190	1.2380	4.0630	1.0300	2.0020	6.1500	2021-06-08_	6/8/21 9:56		AP/MA		
STD4	0.9930	1.4940	1.4940	5.0270	1.2640	2.4850	7.3880	2021-06-08_	6/8/21 10:26		AP/MA		
STD5	1.9750	2.8950	2.8390	9.5610	2.3610	5.1340	14.5440	2021-06-08_	6/8/21 10:56		AP/MA		
STD6	3.9570	5.8540	5.9080	19.5340	4.8250	9.9590	29.2190	2021-06-08_	6/8/21 11:26		AP/MA		
STD7	5.0430	7.6410	7.6170	25.4750	6.4150	12.4850	38.2250	2021-06-08_	6/8/21 11:56		AP/MA		
ICV	1.9730	2.9600	2.8860	9.8620	2.3940	4.9450	14.3090	2021-06-08_	6/8/21 12:33		AP/MA		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-06-08_	6/8/21 13:04		AP/MA		
CCV	2.1530	3.2030	3.2100	10.6050	2.6230	4.5970	15.7920	2021-06-22_	6/22/21 9:34		AP/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-06-22_	6/22/21 10:07		AP/MA		
LB115057BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-06-22_	6/22/21 10:37		AP/MA		
LB115057BSW	2.0670	3.1050	3.1220	10.4710	2.5370	4.7020	15.2480	2021-06-22_	6/22/21 11:07		AP/MA		
M2814-01	0.0000	0.1960	0.0000	0.0000	0.1970	0.0000	0.0000	2021-06-22_	6/22/21 14:26		AP/MA		
M2814-01MS	1.9100	2.8900	2.8780	9.4310	2.3830	3.2950	13.9280	2021-06-22_	6/22/21 15:26		AP/MA		
M2812-07	0.4970	5542.9100	0.0000	2.0060	0.1950	0.0580	89.4290	2021-06-22_	6/22/21 16:26		AP/MA		
M2814-01MSD	1.8110	3.1220	2.8900	9.5000	2.3880	3.9500	14.1610	2021-06-22_	6/22/21 17:26		AP/MA		
CCV	2.0750	3.2160	3.2110	10.6250	2.6160	4.7550	15.7360	2021-06-22_	6/22/21 18:55		AP/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-06-22_	6/22/21 19:25		AP/MA		

CALIBRATION OF COMPONENT F-

Method: ANIONS 06-08-21.mtw
 Equation: $Q = 0.877953 \cdot A - 0.531723$
 RSD: 1.777 %
 Correlation coefficient: 0.999828

TC-1
 6/08/2021
 AM

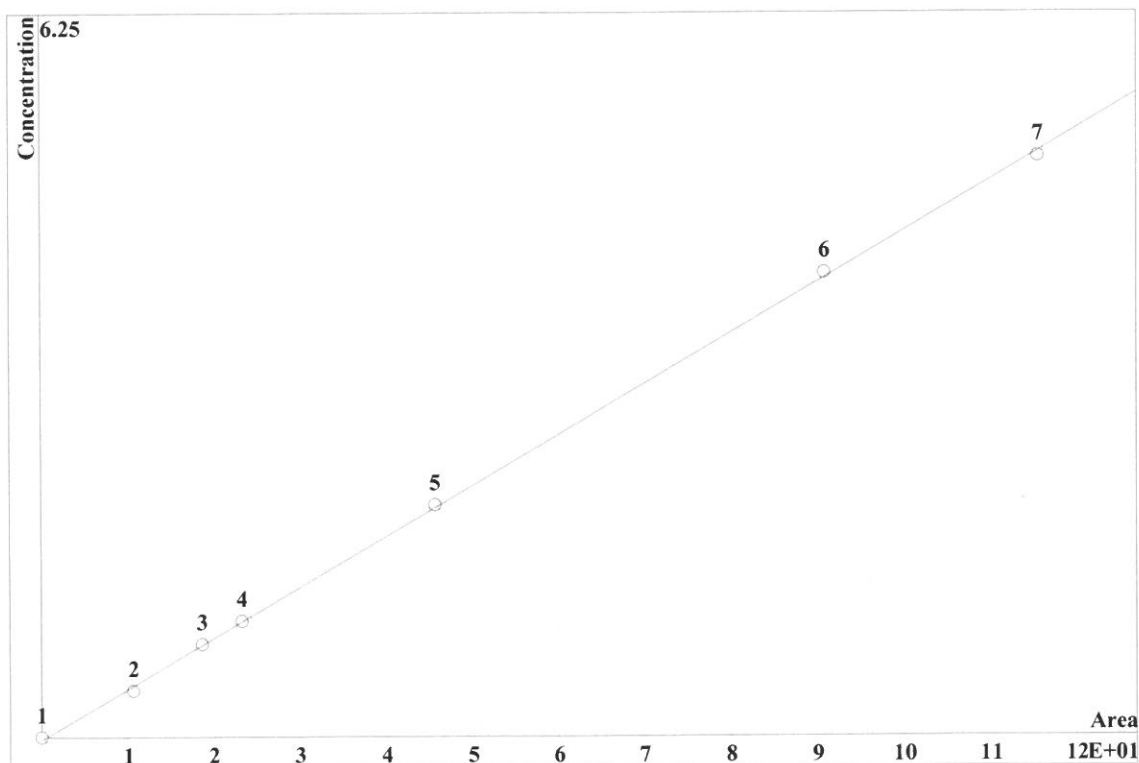


K3 = 0 K2 = 0 K1 = 0.877953 K0 = -0.531723
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.7832	10.65	0.4	20	5.719			Yes
3	1.483	18.63	0.8	20	5.719			Yes
4	1.847	23.24	1	20	5.719			Yes
5	3.72	45.59	2	20	5.719			Yes
6	7.72	90.75	4	20	5.719			Yes
7	9.798	115.5	5	20	5.719			Yes

CALIBRATION OF COMPONENT CL-

Method: ANIONS 06-08-21.mtw
 Equation: $Q = 1.41714 \cdot A + 2.40057$
 RSD: 3.779 %
 Correlation coefficient: 0.999221

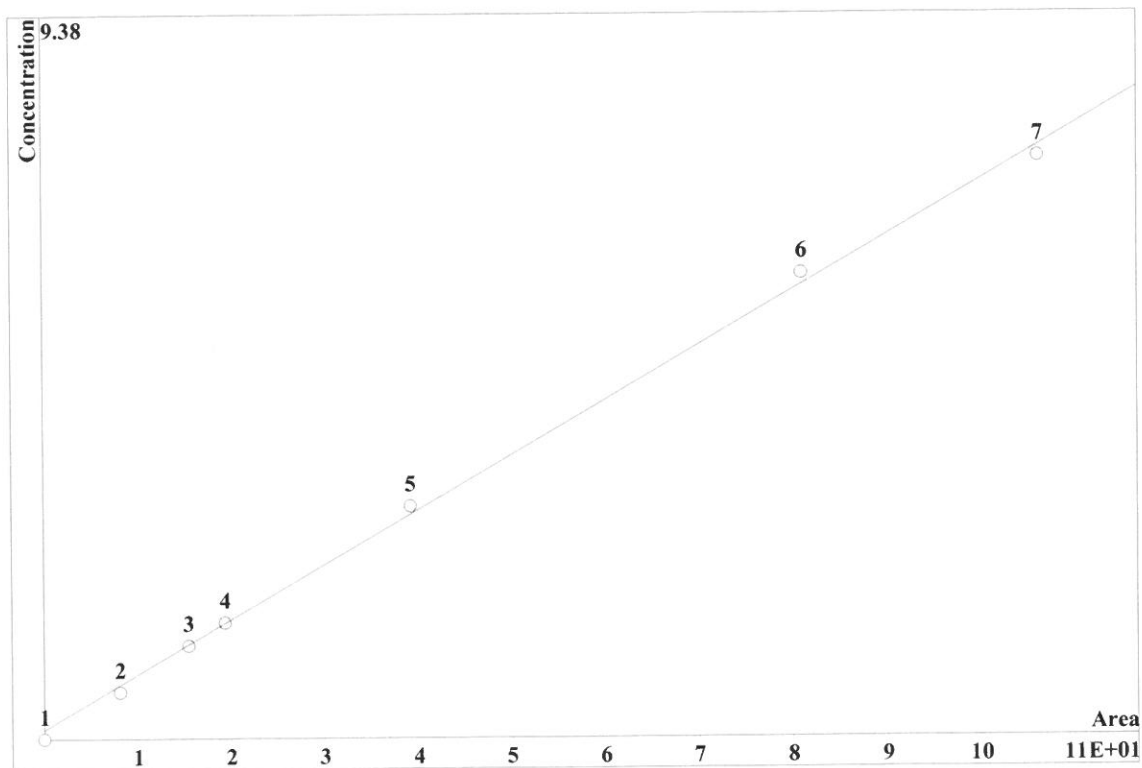


K3 = 0 K2 = 0 K1 = 1.41714 K0 = 2.40057
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0	0	0	No
2	0.6917	8.146	0.6	20	8.802	Yes		Yes
3	1.325	15.51	1.2	20	8.802	Yes		Yes
4	1.669	19.39	1.5	20	8.802	Yes		Yes
5	3.393	39.16	3	20	8.802	Yes		Yes
6	7.171	80.92	6	20	8.802	Yes		Yes
7	9.471	106.1	7.5	20	8.802	Yes		Yes

CALIBRATION OF COMPONENT NO2

Method: ANIONS 06-08-21.mtw
 Equation: $Q = 0.659931 \cdot A + 3.9931$
 RSD: 3.732 %
 Correlation coefficient: 0.999241

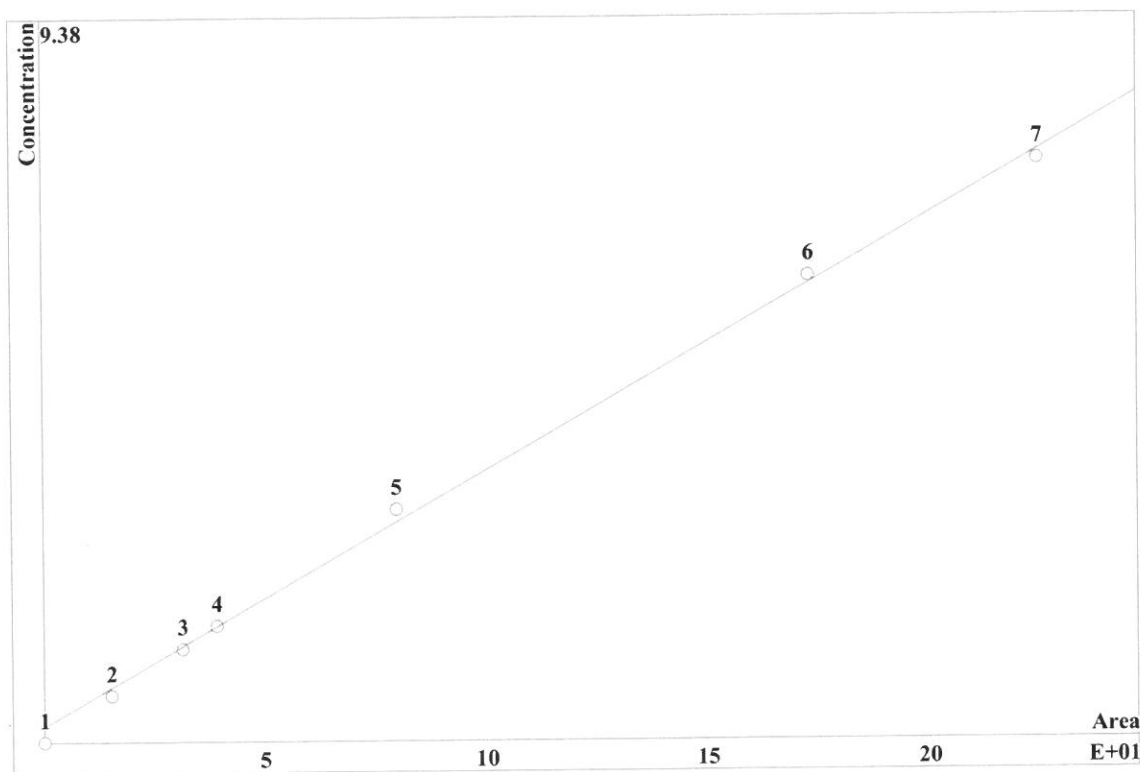


K3 = 0 K2 = 0 K1 = 0.659931 K0 = 3.9931
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	1.034	15.3	0.6	20	10.62			Yes
3	2.107	31.47	1.2	20	10.62			Yes
4	2.621	39.22	1.5	20	10.62			Yes
5	5.241	79.98	3	20	10.62			Yes
6	10.97	173	6	20	10.62			Yes
7	13.94	224.8	7.5	20	10.62			Yes

CALIBRATION OF COMPONENT BR-

Method: ANIONS 06-08-21.mtw
 Equation: $Q = 3.18001 \cdot A + 9.96653$
 RSD: 3.950 %
 Correlation coefficient: 0.999149

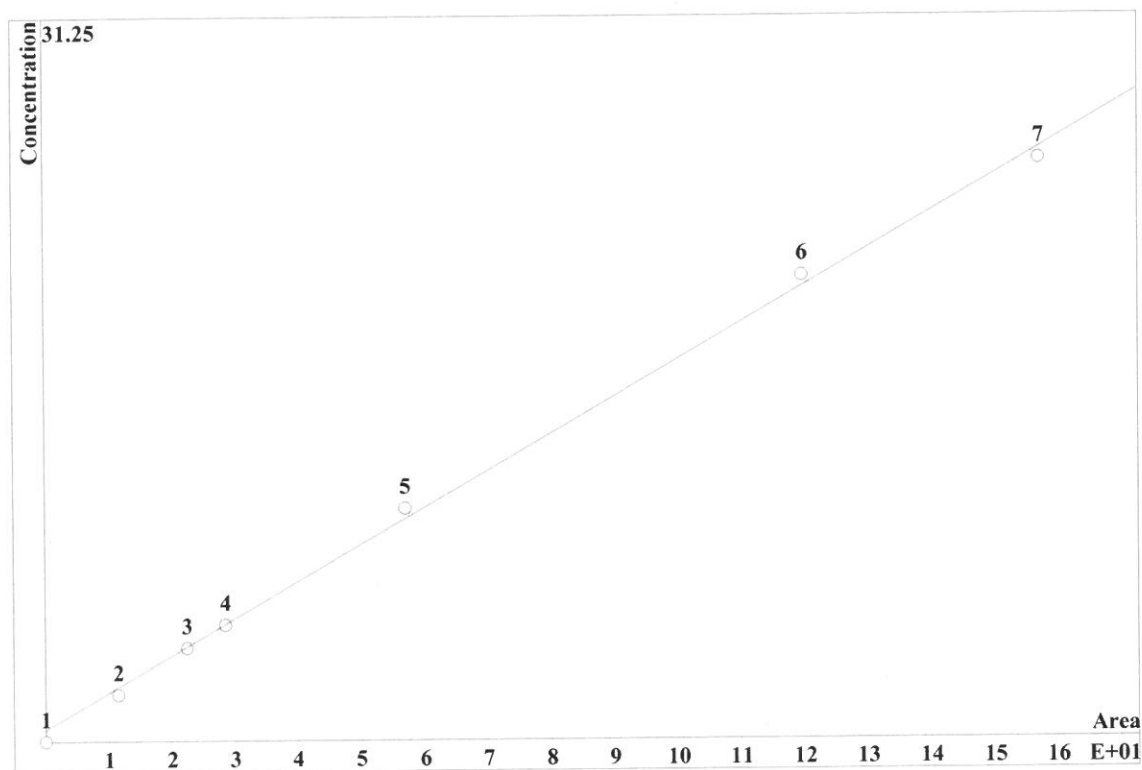


K3 = 0 K2 = 0 K1 = 3.18001 K0 = 9.96653
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.6882	11.57	2	20	13.63			Yes
3	1.372	22.42	4	20	13.63			Yes
4	1.755	28.48	5	20	13.63			Yes
5	3.608	57	10	20	13.63			Yes
6	7.746	119.7	20	20	13.63			Yes
7	10.31	157.1	25	20	13.63			Yes

CALIBRATION OF COMPONENT NO3

Method: ANIONS 06-08-21.mtw
 Equation: $Q = 0.547815 \cdot A + 2.77351$
 RSD: 5.435 %
 Correlation coefficient: 0.998389

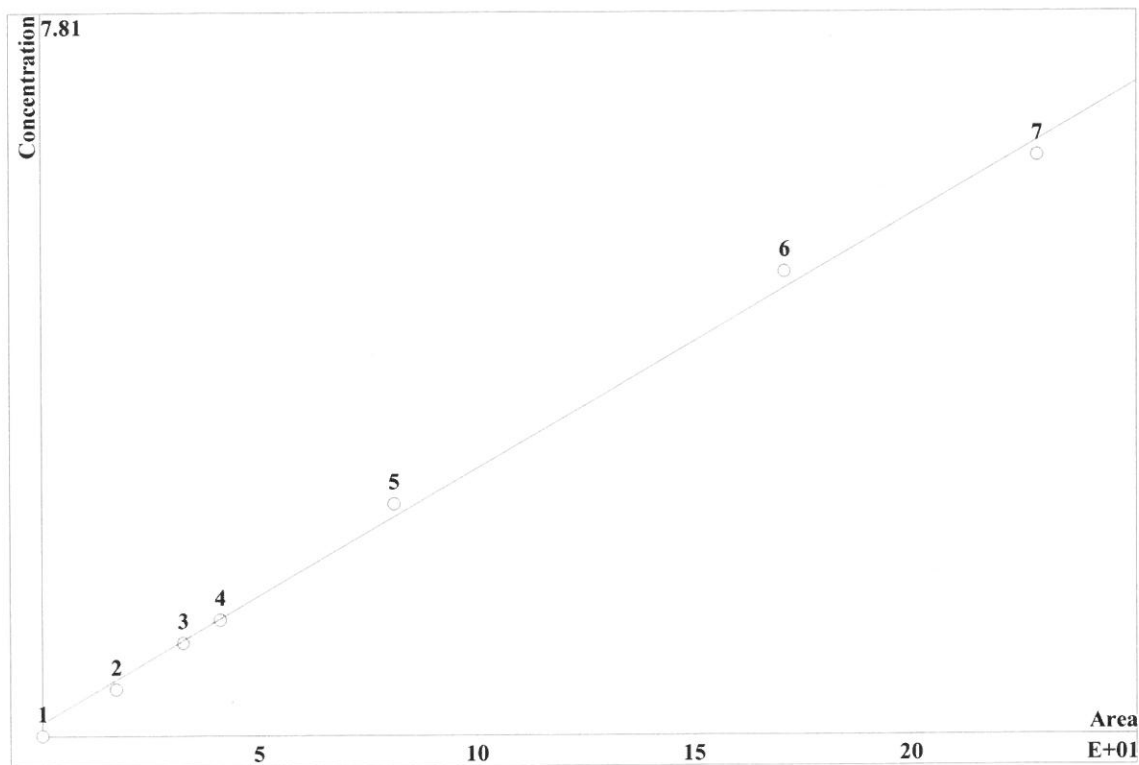


K3 = 0 K2 = 0 K1 = 0.547815 K0 = 2.77351
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.844	17.01	0.5	20	15.72			Yes
3	1.663	32.52	1	20	15.72			Yes
4	2.114	41.1	1.25	20	15.72			Yes
5	4.318	81.14	2.5	20	15.72			Yes
6	9.177	171.1	5	20	15.72			Yes
7	12.26	229.2	6.25	20	15.72			Yes

±□¿\$

CALIBRATION OF COMPONENT HPO4

Method: ANIONS 06-08-21.mtw
 Equation: $Q = 0.987705 \cdot A - 10.2328$
 RSD: 1.420 %
 Correlation coefficient: 0.999890

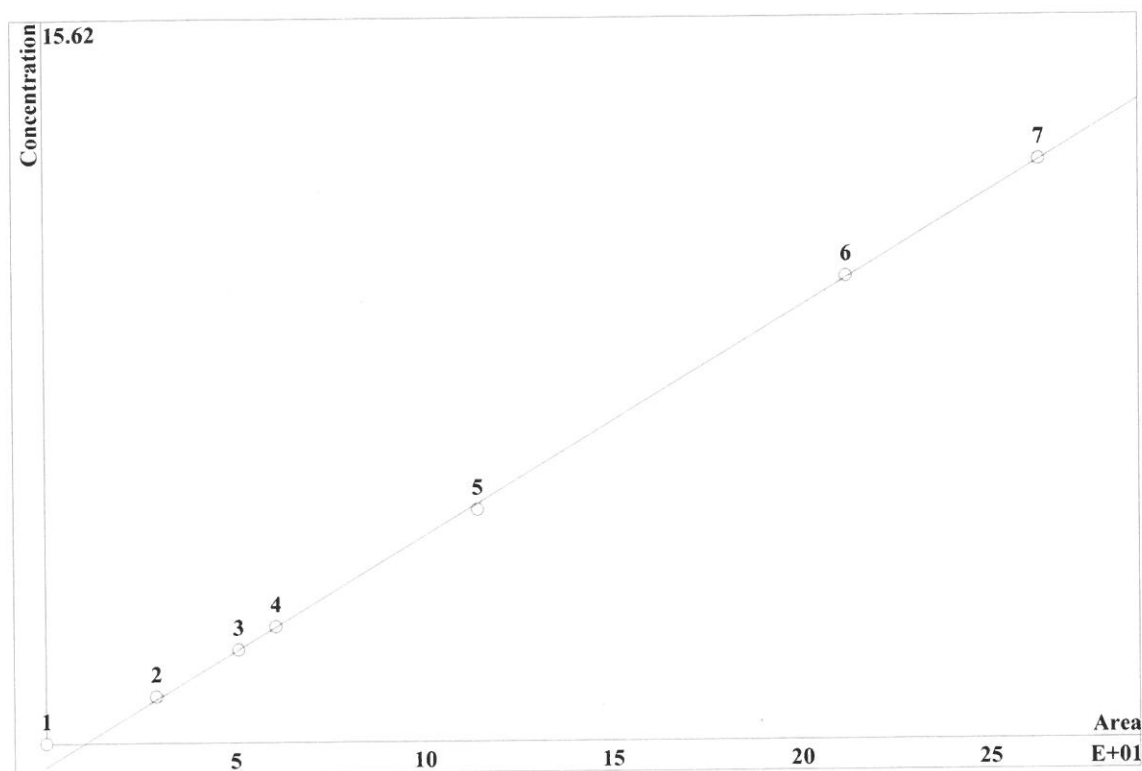


K3 = 0 K2 = 0 K1 = 0.987705 K0 = -10.2328
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.7415	29.29	1	20	21.69			Yes
3	1.318	50.9	2	20	21.69			Yes
4	1.596	60.68	2.5	20	21.69			Yes
5	3.093	114.3	5	20	21.69			Yes
6	6.238	212	10	20	21.69			Yes
7	7.909	263.2	12.5	20	21.69			Yes

CALIBRATION OF COMPONENT SO4

Method: ANIONS 06-08-21.mtw
 Equation: $Q = 1.81758 \cdot A + 14.0332$
 RSD: 3.835 %
 Correlation coefficient: 0.999198

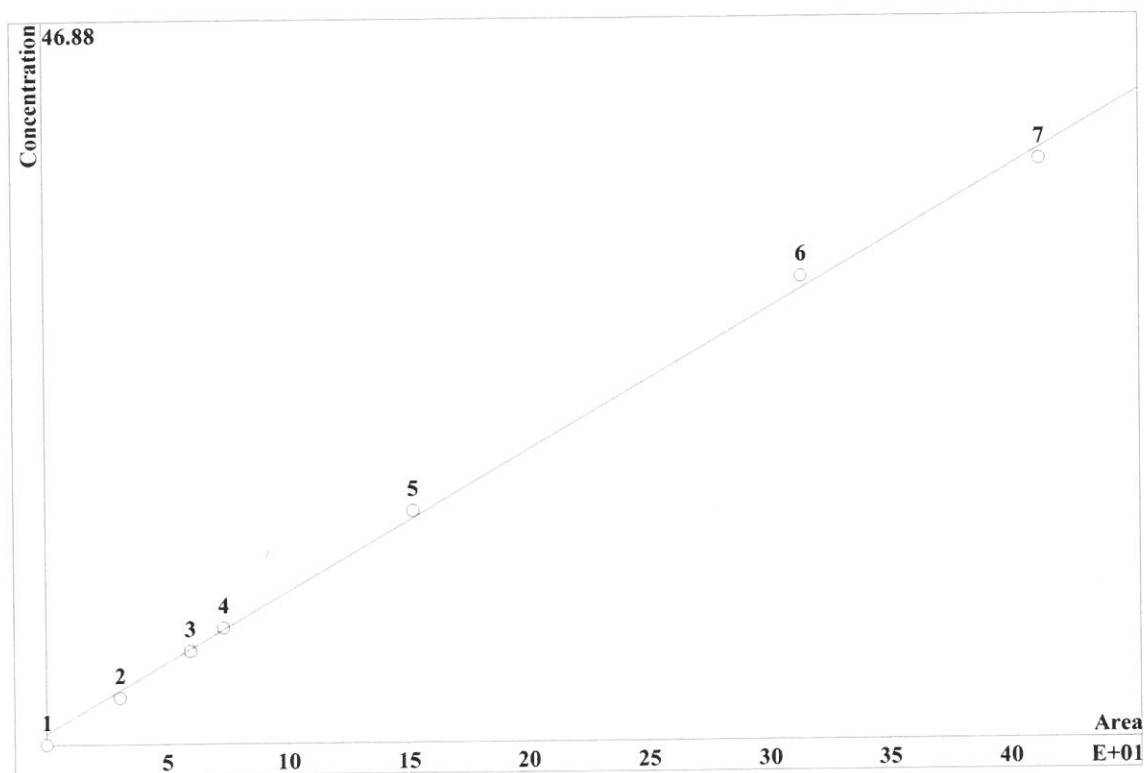

K3 = 0 K2 = 0 K1 = 1.81758 K0 = 14.0332
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	1.102	30.5	3	20	24.84			Yes
3	2.141	59.96	6	20	24.84			Yes
4	2.701	73.58	7.5	20	24.84			Yes
5	5.509	152.3	15	20	24.84			Yes
6	11.7	313.8	30	20	24.84			Yes
7	15.4	412.9	37.5	20	24.84			Yes

Report date: 6/8/2021 4:01:47 PM
Printed by: wet


Ident: STD1
Analysis from: 6/8/2021 8:56:59 AM
File: _2021-06-08_

Last save: 6/8/2021 12:30:16 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74706

Last save: 6/8/2021 11:53:22 AM

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

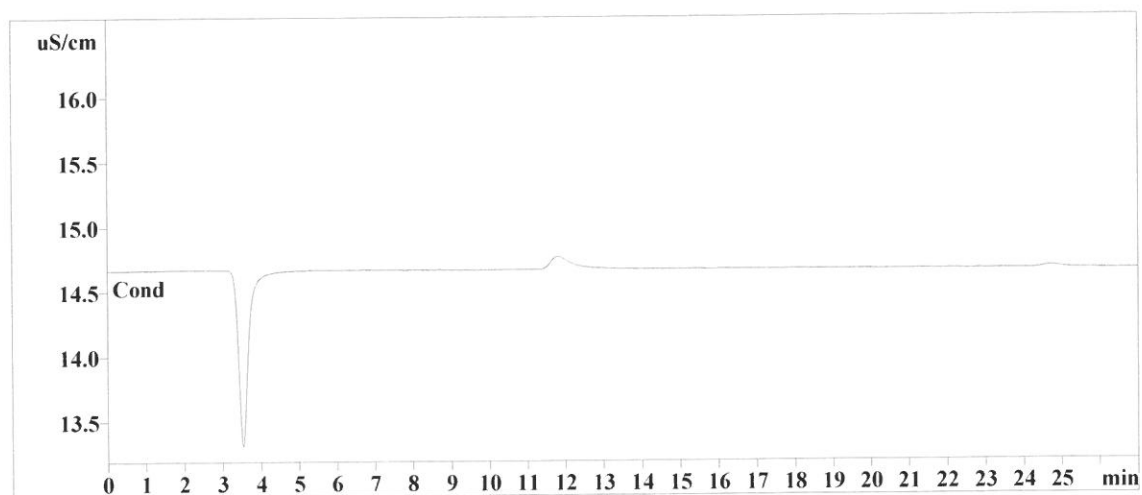

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 6/8/2021 4:01:53 PM
Printed by: wet


Ident: STD2
Analysis from: 6/8/2021 9:26:54 AM
File: _2021-06-08_

Last save: 6/8/2021 12:30:16 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74707

Last save: 6/8/2021 11:53:22 AM

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

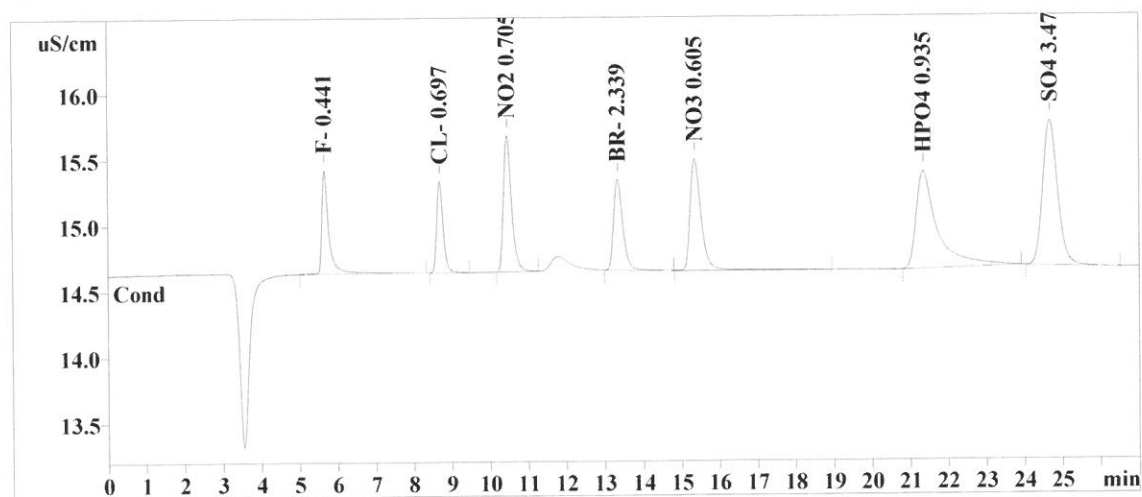

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.66	0.167	0.78	13.30	10.649	8.70	0.
2	8.68	0.176	0.69	11.76	8.146	6.65	0.
3	10.44	0.219	1.03	17.57	15.304	12.50	0.
4	13.33	0.250	0.69	11.69	11.575	9.45	0.
5	15.35	0.290	0.84	14.34	17.013	13.89	0.
6	21.35	0.493	0.74	12.59	29.288	23.91	0.
7	24.67	0.420	1.10	18.70	30.495	24.90	0.
7	27.00	0.288	5.88	99.95	122.471	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/8/2021 4:02:00 PM
Printed by: wet


Ident: STD3
Analysis from: 6/8/2021 9:56:48 AM
File: _2021-06-08_

Last save: 6/8/2021 12:30:18 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74708

Last save: 6/8/2021 11:53:22 AM

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

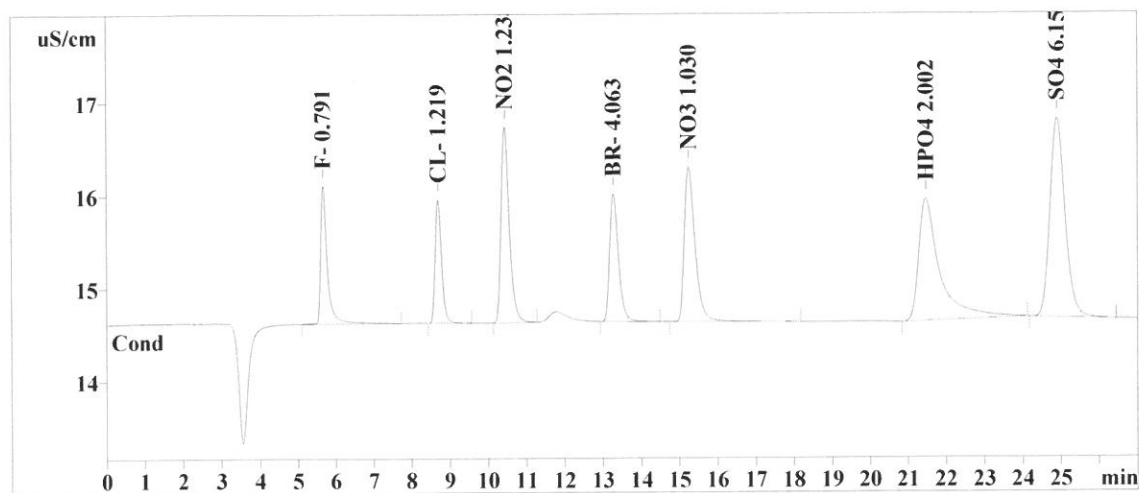

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.67	0.163	1.48	13.00	18.630	8.05	0.
2	8.69	0.175	1.32	11.61	15.513	6.70	0.
3	10.43	0.221	2.11	18.46	31.468	13.60	0.
4	13.27	0.245	1.37	12.03	22.421	9.69	0.
5	15.24	0.286	1.66	14.58	32.524	14.05	0.
6	21.47	0.489	1.32	11.54	50.901	22.00	0.
7	24.90	0.427	2.14	18.76	59.956	25.91	0.
7	27.00	0.287	11.41	99.97	231.414	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/8/2021 4:02:06 PM
Printed by: wet


Ident: STD4
Analysis from: 6/8/2021 10:26:43 AM
File: _2021-06-08_

Last save: 6/8/2021 12:30:18 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74709

Last save: 6/8/2021 11:53:22 AM

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

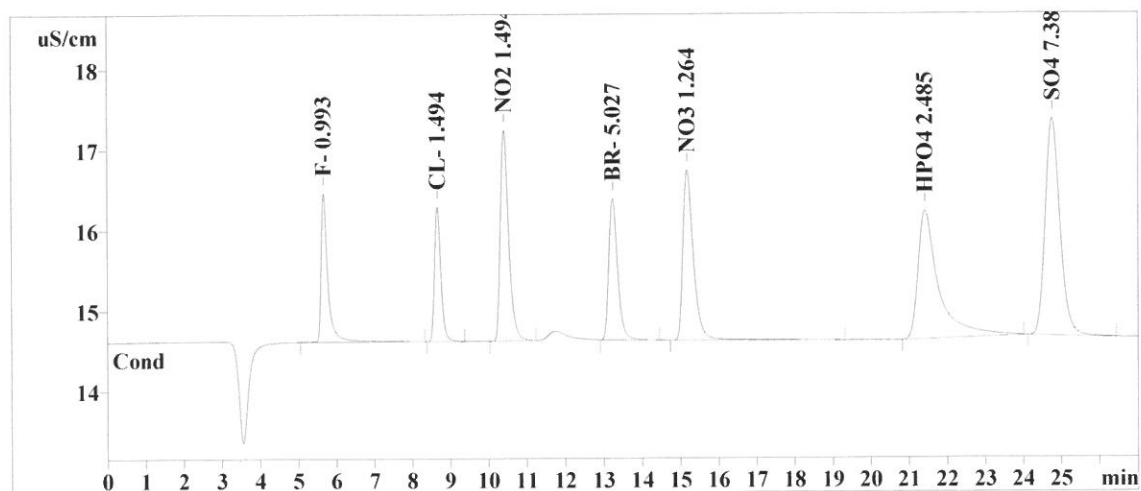

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.67	0.163	1.85	12.91	23.236	8.13	0.
2	8.66	0.174	1.67	11.67	19.386	6.79	0.
3	10.40	0.221	2.62	18.33	39.225	13.73	0.
4	13.22	0.243	1.75	12.27	28.485	9.97	0.
5	15.17	0.283	2.11	14.77	41.096	14.39	0.
6	21.41	0.480	1.60	11.16	60.679	21.24	0.
7	24.76	0.413	2.70	18.88	73.578	25.75	0.
7	27.00	0.283	14.30	99.99	285.685	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/8/2021 4:02:12 PM
Printed by: wet


Ident: STD5
Analysis from: 6/8/2021 10:56:39 AM
File: _2021-06-08_

Last save: 6/8/2021 12:30:18 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74710

Last save: 6/8/2021 11:53:22 AM

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

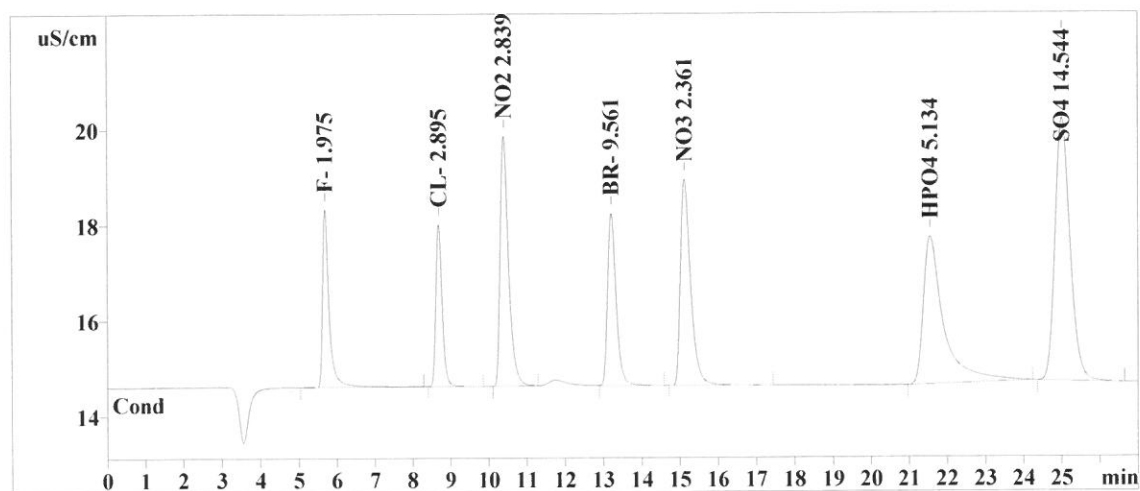

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.69	0.162	3.72	12.88	45.591	8.01	0.
2	8.68	0.173	3.39	11.75	39.163	6.88	0.
3	10.40	0.225	5.24	18.14	79.977	14.04	0.
4	13.20	0.236	3.61	12.49	56.998	10.01	0.
5	15.12	0.279	4.32	14.95	81.144	14.25	0.
6	21.56	0.471	3.09	10.71	114.321	20.07	0.
7	25.01	0.421	5.51	19.07	152.321	26.75	0.
7	27.00	0.281	28.88	99.99	569.516	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/8/2021 4:02:18 PM
Printed by: wet


Ident: STD6
Analysis from: 6/8/2021 11:26:34 AM
File: _2021-06-08_

Last save: 6/8/2021 12:30:18 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74711

Last save: 6/8/2021 11:53:22 AM

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

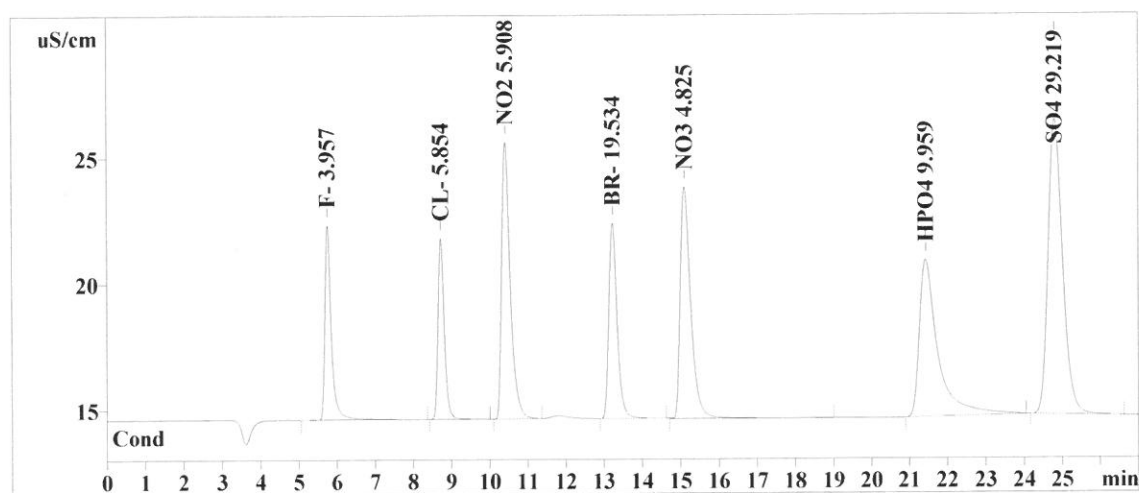

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.76	0.159	7.72	12.71	90.746	7.81	0.
2	8.72	0.168	7.17	11.81	80.919	6.97	0.
3	10.40	0.232	10.97	18.06	172.992	14.90	0.
4	13.23	0.231	7.75	12.76	119.723	10.31	0.
5	15.10	0.275	9.18	15.11	171.083	14.73	0.
6	21.43	0.443	6.24	10.27	212.011	18.26	0.
7	24.80	0.407	11.70	19.27	313.793	27.02	0.
7	27.00	0.274	60.72	100.00	1161.266	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/8/2021 4:02:23 PM
Printed by: wet


Ident: STD7
Analysis from: 6/8/2021 11:56:29 AM
File: _2021-06-08_

Last save: 6/8/2021 12:30:18 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74712

Last save: 6/8/2021 11:53:22 AM

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

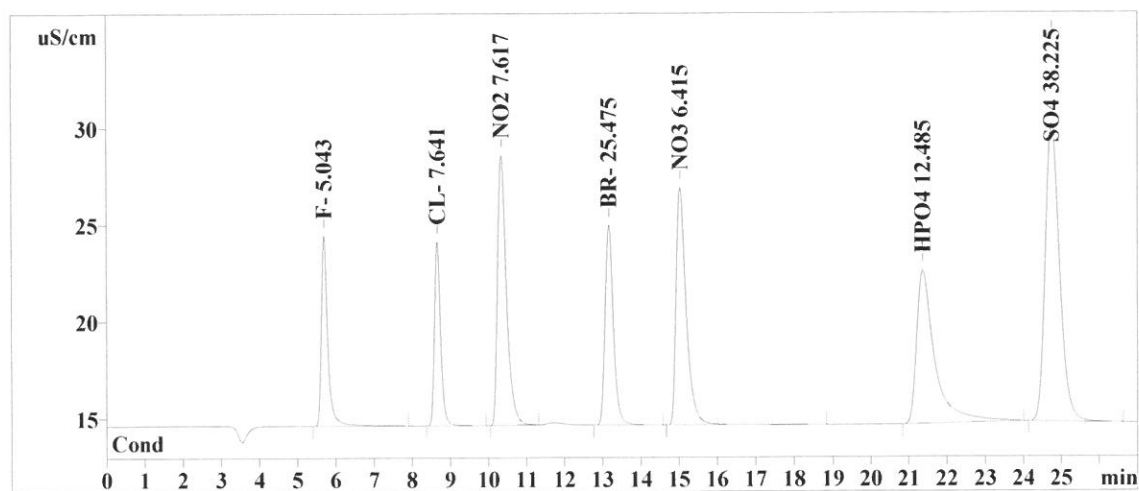

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.70	0.162	9.80	12.39	115.481	7.65	0.
2	8.66	0.167	9.47	11.97	106.145	7.04	0.
3	10.33	0.237	13.94	17.62	224.791	14.90	0.
4	13.16	0.228	10.31	13.04	157.087	10.41	0.
5	15.03	0.276	12.26	15.50	229.156	15.19	0.
6	21.37	0.437	7.91	10.00	263.177	17.44	0.
7	24.74	0.408	15.40	19.47	412.890	27.37	0.
7	27.00	0.274	79.08	100.00	1508.728	100.00	0.

This report has been created by IC Net
METROHM LTD

Date - 6/8/2021

Instrument ID - IC-1

Analyst - AM

Anion Calibration std - relative error calculations, acceptance limit is -30 to 30 for std 2 and -10 to 10 for other std																		
Parameter	TV of std2	Result of std2	% RE std2	TV of std3	Result of std3	% RE std3	TV of std4	Result of std4	% RE std4	TV of std5	Result of std5	% RE std5	TV of std6	Result of std6	% RE std6	TV of std7	Result of std7	% RE std7
F	0.4	0.441	10.3	0.8	0.791	-1.1	1	0.993	-0.7	2	1.975	-1.3	4	3.957	-1.1	5	5.043	0.9
CL	0.6	0.697	16.2	1.2	1.219	1.6	1.5	1.494	-0.4	3	2.895	-3.5	6	5.854	-2.4	7.5	7.641	1.9
NO2	0.6	0.705	17.5	1.2	1.238	3.2	1.5	1.494	-0.4	3	2.839	-5.4	6	5.908	-1.5	7.5	7.617	1.6
BR	2	2.339	17.0	4	4.063	1.6	5	5.027	0.5	10	9.561	-4.4	20	19.534	-2.3	25	25.475	1.9
NO3	0.5	0.605	21.0	1	1.030	3.0	1.25	1.264	1.1	2.5	2.361	-5.6	5	4.825	-3.5	6.25	6.415	2.6
HPO4	1	0.935	-6.5	2	2.002	0.1	2.5	2.485	-0.6	5	5.134	2.7	10	9.959	-0.4	12.5	12.485	-0.1
SO4	3	3.473	15.8	6	6.150	2.5	7.5	7.388	-1.5	15	14.544	-3.0	30	29.219	-2.6	37.5	38.225	1.9

06/08/2021
AM

Report date: 6/8/2021 4:03:13 PM
 Printed by: wet


Ident: ICV
 Analysis from: 6/8/2021 12:33:12 PM
 File: _2021-06-08_

Last save: 6/8/2021 1:00:02 PM

Method: ANIONS 06-08-21.mtw
 Run operator: wet
 Analysis number: 74713

Last save: 6/8/2021 12:23:18 PM

SAMPLE:
 : AM/AP
 Vial number: 9
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

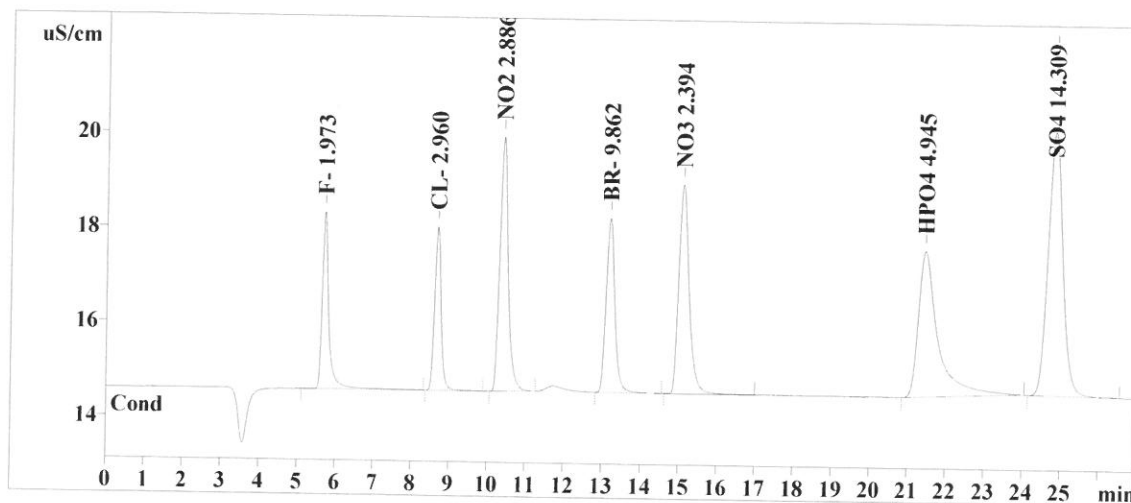

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.70	0.162	3.73	12.75	45.544	8.01	0.
2	8.67	0.174	3.44	11.77	40.082	7.05	0.
3	10.37	0.224	5.36	18.33	81.398	14.32	0.
4	13.16	0.241	3.67	12.55	58.891	10.36	0.
5	15.07	0.277	4.41	15.07	82.350	14.49	0.
6	21.44	0.460	3.07	10.48	110.495	19.44	0.
7	24.80	0.409	5.57	19.03	149.733	26.34	0.
7	27.00	0.278	29.24	100.00	568.494	100.00	0.

This report has been created by IC Net
 METROHM LTD

Report date: 6/8/2021 4:03:19 PM
Printed by: wet


Ident: ICB
Analysis from: 6/8/2021 1:04:39 PM
File: _2021-06-08_

Last save: 6/8/2021 1:31:28 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74714

Last save: 6/8/2021 12:23:18 PM

SAMPLE:
: AM/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

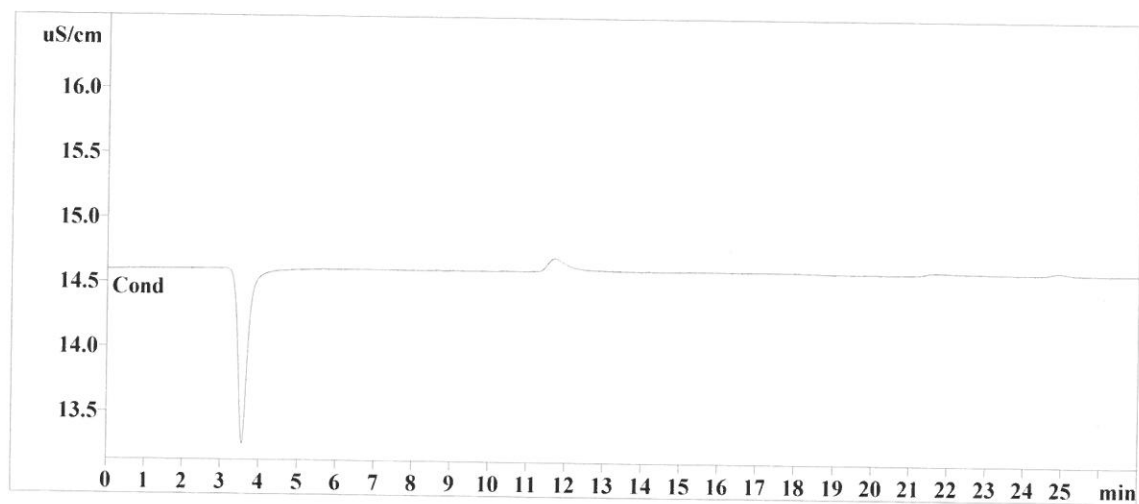

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:44:32 AM
Printed by: wet


Ident: CCV
Analysis from: 6/22/2021 9:34:33 AM
File: _2021-06-22_

Last save: 6/22/2021 10:01:22 AM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74817

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

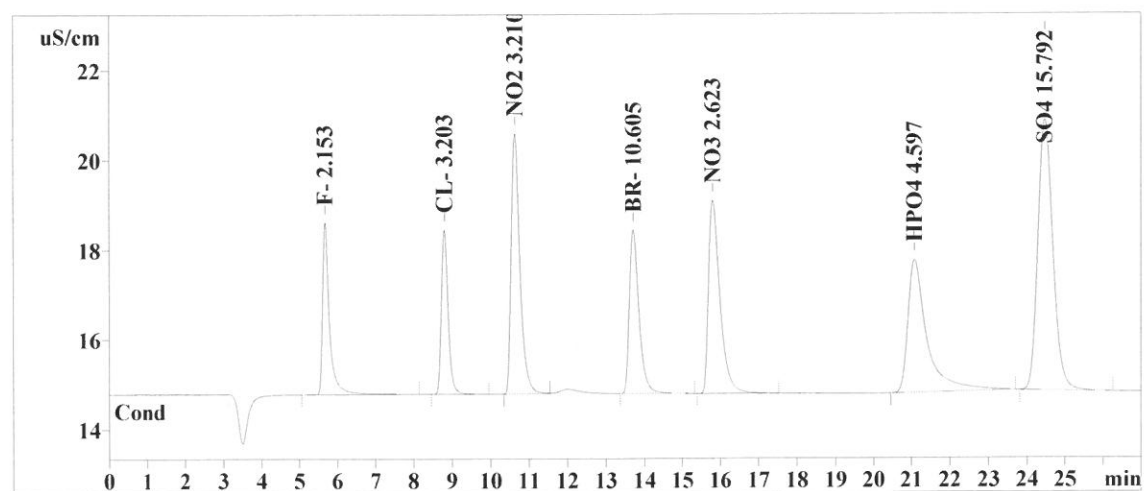

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.67	0.169	3.83	12.67	49.661	8.17	0.
2	8.80	0.177	3.65	12.09	43.510	7.15	0.
3	10.62	0.232	5.80	19.17	91.219	15.00	0.
4	13.71	0.258	3.64	12.06	63.565	10.45	0.
5	15.80	0.310	4.30	14.22	90.700	14.91	0.
6	21.09	0.454	2.96	9.79	103.443	17.01	0.
7	24.46	0.417	6.04	20.00	166.049	27.30	0.
7	27.00	0.288	30.22	100.00	608.147	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:44:41 AM
Printed by: wet


Ident: CCB
Analysis from: 6/22/2021 10:07:54 AM
File: _2021-06-22_

Last save: 6/22/2021 10:34:44 AM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74818

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

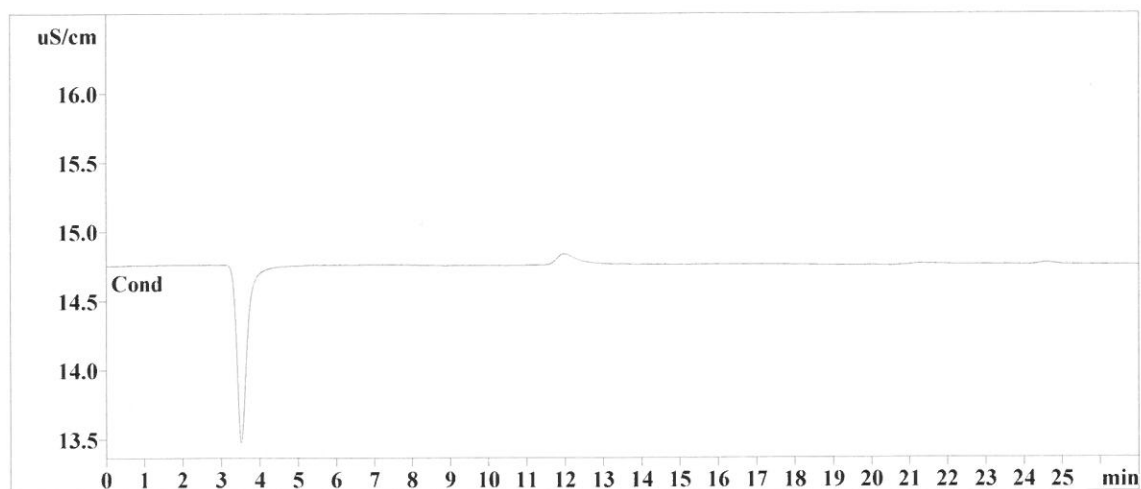

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:44:47 AM
Printed by: wet


Ident: LB115057BLW
Analysis from: 6/22/2021 10:37:49 AM
File: _2021-06-22_

Last save: 6/22/2021 4:00:50 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74819

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

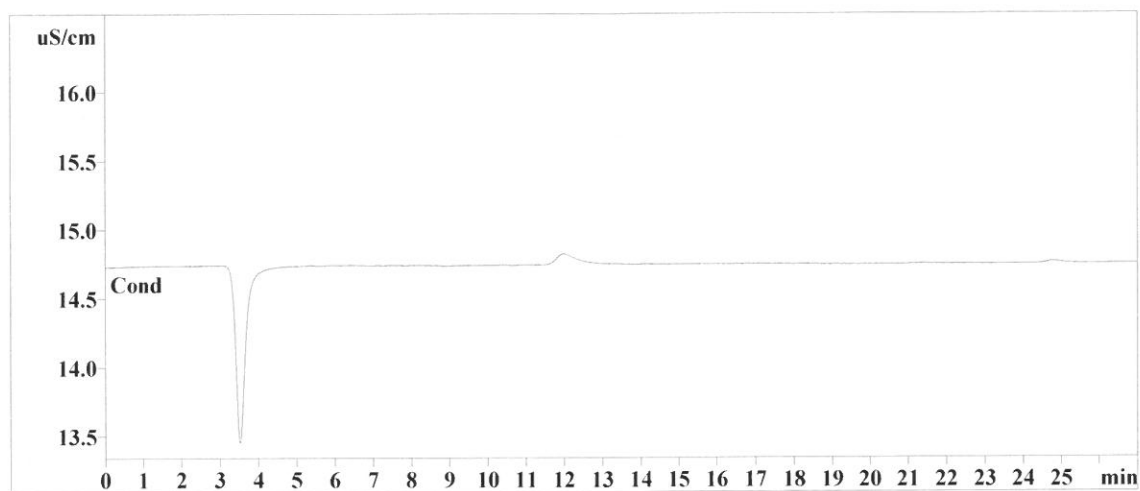

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:44:55 AM
Printed by: wet


Ident: LB115057BSW
Analysis from: 6/22/2021 11:07:44 AM
File: _2021-06-22_

Last save: 6/22/2021 4:00:50 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74820

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

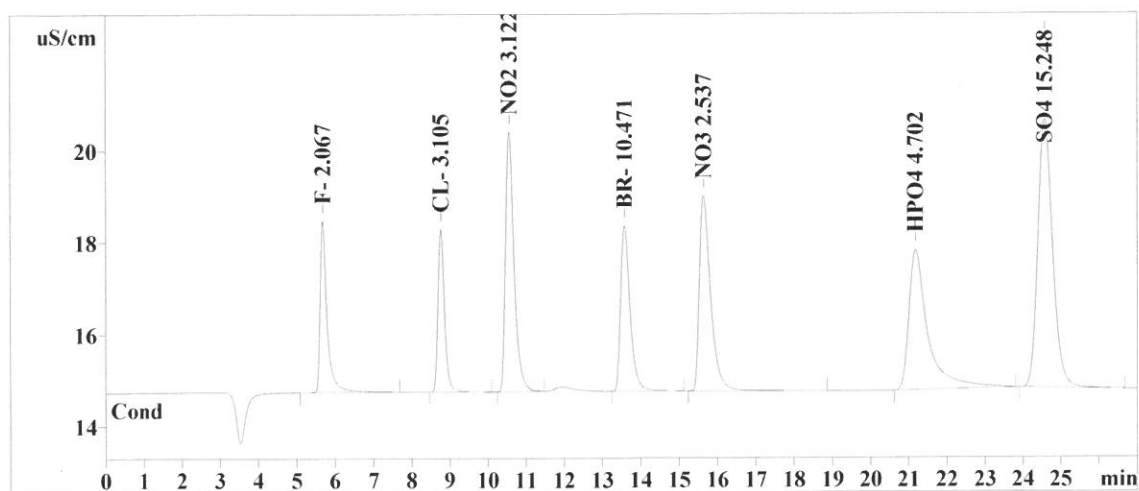

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.68	0.169	3.72	12.55	47.699	8.03	0.
2	8.76	0.177	3.53	11.92	42.121	7.09	0.
3	10.55	0.231	5.65	19.06	88.575	14.90	0.
4	13.58	0.259	3.60	12.14	62.719	10.55	0.
5	15.63	0.303	4.24	14.31	87.566	14.73	0.
6	21.18	0.450	3.04	10.27	105.576	17.76	0.
7	24.57	0.414	5.85	19.75	160.064	26.93	0.
7	27.00	0.286	29.64	100.00	594.321	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:45:03 AM
Printed by: wet


Ident: M2814-01
Analysis from: 6/22/2021 2:26:39 PM
File: _2021-06-22_

Last save: 6/22/2021 2:53:28 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74823

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

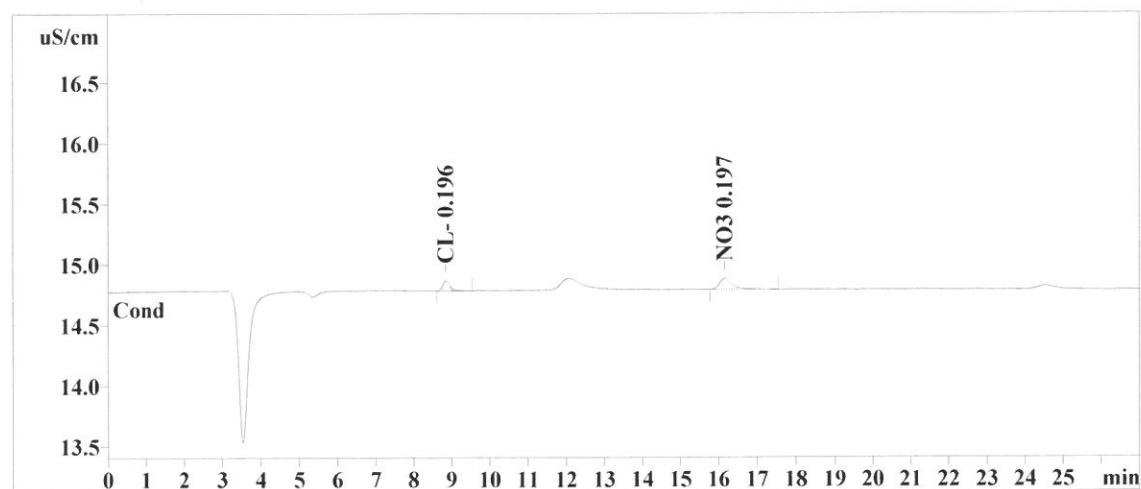

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	0.00	0.000	0.00	0.00	0.000	0.00	0.
2	8.84	0.188	0.08	47.78	1.071	33.41	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	0.00	0.000	0.00	0.00	0.000	0.00	0.
5	16.15	0.332	0.09	51.94	2.135	66.59	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	27.00	0.074	0.17	99.72	3.206	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:47:26 AM
Printed by: wet


Ident: M2814-01MS
Analysis from: 6/22/2021 3:26:29 PM
File: _2021-06-22_

Last save: 6/23/2021 9:47:18 AM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74825

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

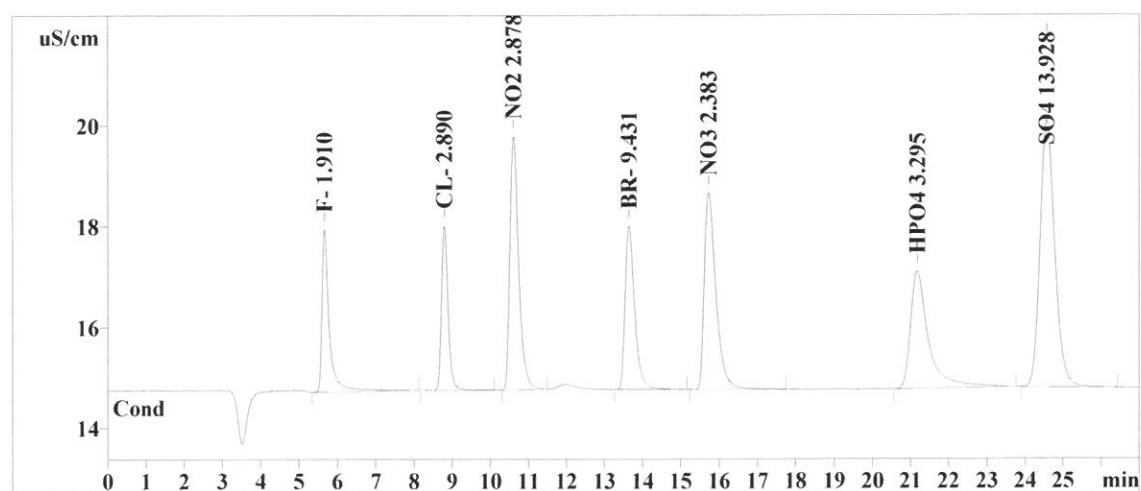

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.67	0.170	3.22	12.27	44.111	8.40	0.
2	8.78	0.178	3.25	12.39	39.098	7.45	0.
3	10.59	0.240	5.02	19.14	81.173	15.46	0.
4	13.64	0.257	3.24	12.33	56.180	10.70	0.
5	15.72	0.309	3.90	14.86	81.921	15.60	0.
6	21.17	0.439	2.32	8.85	77.071	14.68	0.
7	24.56	0.417	5.29	20.15	145.540	27.72	0.
7	27.00	0.287	26.25	99.99	525.094	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:48:09 AM
Printed by: wet


Ident: M2812-07
Analysis from: 6/22/2021 4:26:20 PM
File: _2021-06-22_

Last save: 6/23/2021 9:48:02 AM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74827

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

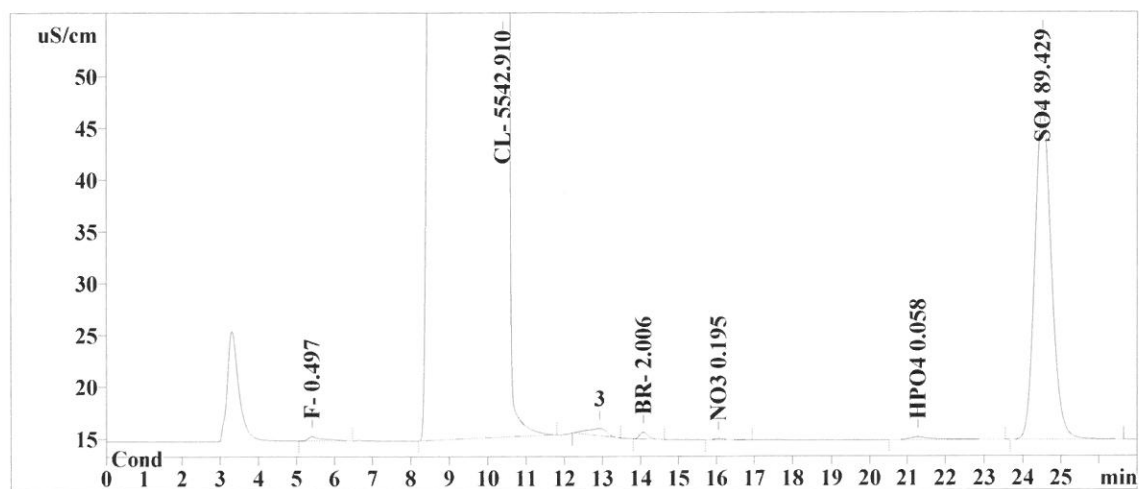

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.41	0.303	0.43	0.04	11.937	0.02	0.
2	10.37	1.471	962.46	96.53	78225.249	98.69	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	14.07	0.224	0.65	0.07	9.482	0.01	0.
5	16.05	0.294	0.10	0.01	2.040	0.00	0.
6	21.28	0.523	0.27	0.03	11.532	0.01	0.
7	24.51	0.463	32.21	3.23	976.317	1.23	0.
7	27.00	0.468	996.12	99.91	79236.557	99.97	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:48:23 AM
Printed by: wet


Ident: M2814-01MSD
Analysis from: 6/22/2021 5:26:10 PM
File: _2021-06-22_

Last save: 6/22/2021 5:53:00 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74829

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

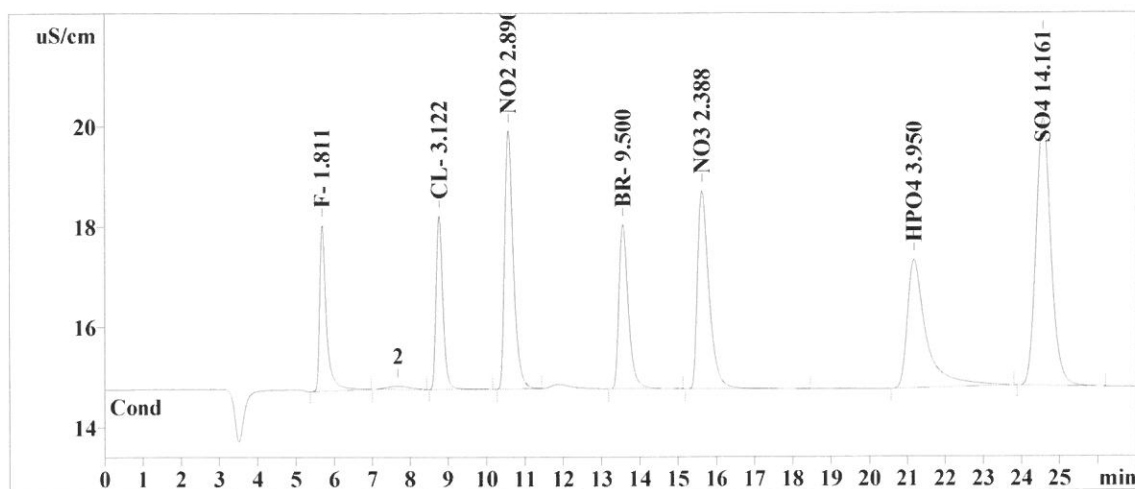

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.68	0.169	3.31	12.23	41.867	7.67	0.
2	8.76	0.182	3.45	12.75	42.370	7.77	0.
3	10.56	0.236	5.14	18.98	81.521	14.94	0.
4	13.56	0.257	3.27	12.07	56.612	10.38	0.
5	15.61	0.306	3.94	14.56	82.115	15.05	0.
6	21.17	0.456	2.56	9.46	90.347	16.56	0.
7	24.56	0.422	5.34	19.71	148.098	27.14	0.
7	27.00	0.290	27.02	99.76	542.930	99.50	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:48:31 AM
Printed by: wet


Ident: CCV
Analysis from: 6/22/2021 6:55:55 PM
File: _2021-06-22_

Last save: 6/22/2021 7:22:44 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74832

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

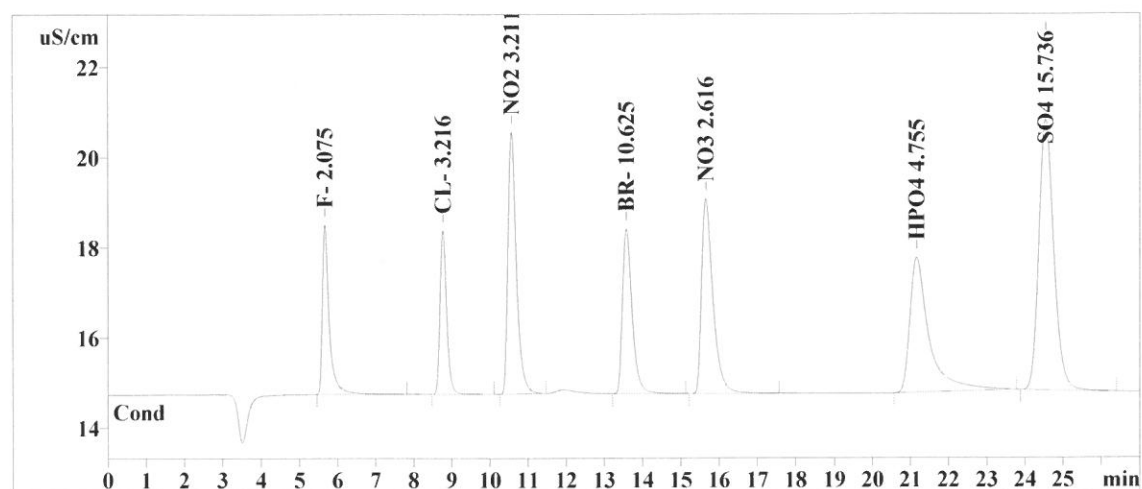

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.67	0.171	3.75	12.44	47.882	7.86	0.
2	8.76	0.179	3.62	12.01	43.690	7.17	0.
3	10.56	0.233	5.81	19.27	91.274	14.99	0.
4	13.58	0.260	3.65	12.10	63.691	10.46	0.
5	15.65	0.309	4.32	14.32	90.439	14.85	0.
6	21.16	0.461	2.99	9.93	106.653	17.51	0.
7	24.54	0.418	6.01	19.93	165.429	27.16	0.
7	27.00	0.290	30.14	100.00	609.058	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 6/23/2021 9:48:41 AM
Printed by: wet


Ident: CCB
Analysis from: 6/22/2021 7:25:50 PM
File: _2021-06-22_

Last save: 6/22/2021 7:52:40 PM

Method: ANIONS 06-08-21.mtw
Run operator: wet
Analysis number: 74833

Last save: 6/18/2021 10:15:14 AM

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

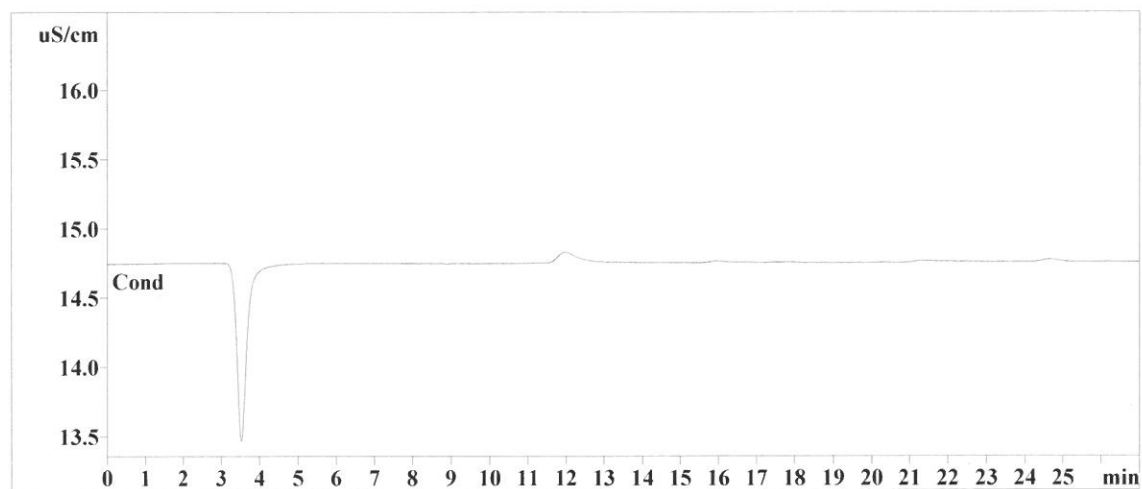

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD