


7470A

LB115104

INSTRUMENT ID: CVL

Linear

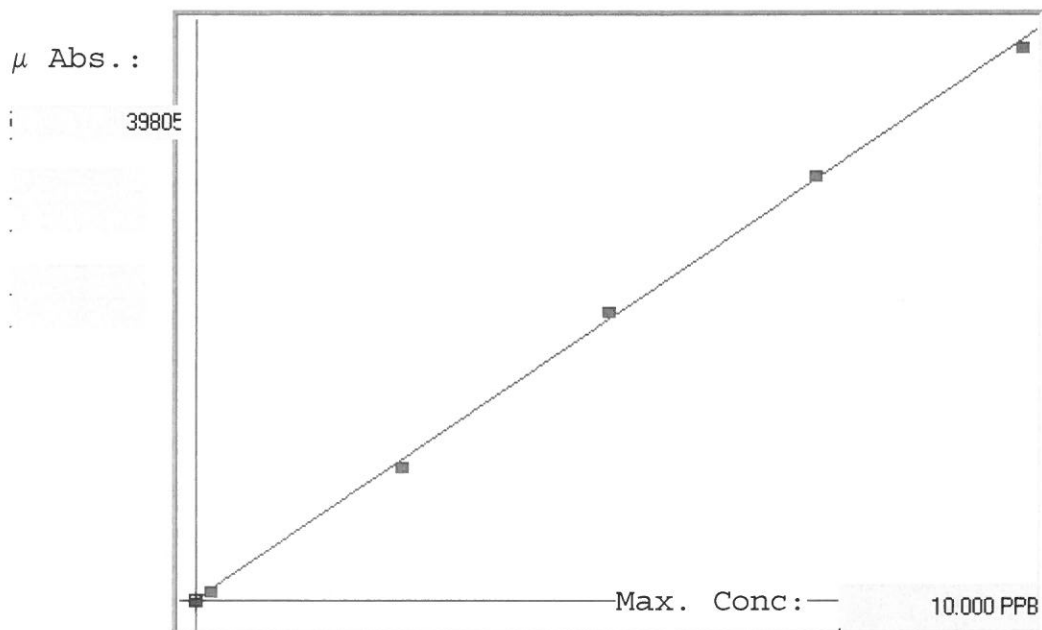

A= 0.0000e+000

B= 2.4825e-004

C= -5.7832e-003

Rho= 0.9996287

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	9/10/1
0.0	0.000	-0.000	-0.000	22	0.000	22					-
0.2	0.200	0.188	-0.012	779	0.0 %	779					-6
2.5	2.500	2.390	-0.110	9649	0.0 %	9649					-4
5.0	5.000	5.158	0.158	20801	0.0 %	20801					3
7.5	7.500	7.589	0.089	30593	0.0 %	30593					1
10.0	10.000	9.876	-0.124	39805	0.0 %	39805					-1

LB115104 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 25 Jun 2021 13:24:42							
Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type		
0.0 - 1	50	22	-	0.00007470A	PPB		25 Jun 2021 13:39:13	S	Std		
0.2 - 1	50.2	779	-	0.20007470A	PPB		25 Jun 2021 13:41:30	S	Std		
2.5 - 1	52.5	9649	-	2.50007470A	PPB		25 Jun 2021 13:43:46	S	Std		
5.0 - 1	55	20801	-	5.00007470A	PPB		25 Jun 2021 13:46:03	S	Std		
7.5 - 1	57.5	30593	-	7.50007470A	PPB		25 Jun 2021 13:48:20	S	Std		
10.0 - 1	510	39805	-	10.00007470A	PPB		25 Jun 2021 13:50:35	S	Std		
ICV78 - 1	ICV78	14848	3.6803	-7470A	PPB		25 Jun 2021 13:53:29	U	SMPL		
ICB78 - 1	ICB78	-98	-0.0301	-7470A	PPB		25 Jun 2021 13:55:43	U	SMPL		
CCV67 - 1	CCV67	20011	4.9620	-7470A	PPB		25 Jun 2021 13:57:58	U	SMPL		
CCB67 - 1	CCB67	-122	-0.0361	-7470A	PPB		25 Jun 2021 14:00:13	U	SMPL		
CRA - 1	CRA	707	0.1697	-7470A	PPB		25 Jun 2021 14:02:28	U	SMPL		
HighStd - 1	HighStd	40088	9.9462	-7470A	PPB		25 Jun 2021 14:04:43	U	SMPL		
ChkStd - 1	ChkStd	28144	6.9811	-7470A	PPB		25 Jun 2021 14:06:58	U	SMPL		
PB137342BL - 1	PBW	-169	-0.0477	-7470A	PPB		25 Jun 2021 14:09:14	U	SMPL		
PB137342BS - 1	LCSW	16430	4.0730	-7470A	PPB		25 Jun 2021 14:11:30	U	SMPL		
M2812-02 - 1	356-349	-98	-0.0301	-7470A	PPB		25 Jun 2021 14:13:46	U	SMPL		
M2812-02DUP - 1	356-349DUP	-20	-0.0107	-7470A	PPB		25 Jun 2021 14:16:03	U	SMPL		
M2812-02MS - 1	356-349MS	15002	3.7185	-7470A	PPB		25 Jun 2021 14:18:19	U	SMPL		
M2812-02MSD - 1	356-349MSD	16668	4.1321	-7470A	PPB		25 Jun 2021 14:20:36	U	SMPL		
M2812-05 - 1	293-347	-89	-0.0279	-7470A	PPB		25 Jun 2021 14:22:52	U	SMPL		
CCV68 - 1	CCV68	20121	4.9893	-7470A	PPB		25 Jun 2021 14:25:07	U	SMPL		
CCB68 - 1	CCB68	-103	-0.0314	-7470A	PPB		25 Jun 2021 14:27:23	U	SMPL		
M2824-03 - 1	ABN-1	0	-0.0058	-7470A	PPB		25 Jun 2021 14:29:38	U	SMPL		
M2826-01 - 1	SS-1(SLUDGE)	524	0.1243	-7470A	PPB		25 Jun 2021 14:31:54	U	SMPL		
M2829-07 - 1	15B-STOCKPILE-1	14	-0.0023	-7470A	PPB		25 Jun 2021 14:34:08	U	SMPL		
M2829-08 - 1	15B-STOCKPILE-2A	10	-0.0033	-7470A	PPB		25 Jun 2021 14:36:23	U	SMPL		
M2829-09 - 1	15B-STOCKPILE-2B	23	-0.0001	-7470A	PPB		25 Jun 2021 14:38:39	U	SMPL		
M2829-10 - 1	15B-STOCKPILE-3A	16	-0.0018	-7470A	PPB		25 Jun 2021 14:40:55	U	SMPL		
M2829-11 - 1	15B-STOCKPILE-3B	16	-0.0018	-7470A	PPB		25 Jun 2021 14:43:12	U	SMPL		
M2829-12 - 1	15B-DUP-01	16	-0.0018	-7470A	PPB		25 Jun 2021 14:45:29	U	SMPL		
M2832-02 - 1	TP-3-WC	15	-0.0021	-7470A	PPB		25 Jun 2021 14:47:45	U	SMPL		
M2846-02 - 1	1-4-FEET-TP	32	0.0022	-7470A	PPB		25 Jun 2021 14:50:01	U	SMPL		
CCV69 - 1	CCV69	19515	4.8389	-7470A	PPB		25 Jun 2021 14:52:16	U	SMPL		
CCB69 - 1	CCB69	-92	-0.0286	-7470A	PPB		25 Jun 2021 14:54:32	U	SMPL		
M2852-02 - 1	MANHOLE-WC-S	5	-0.0045	-7470A	PPB		25 Jun 2021 14:56:47	U	SMPL		
M2852-05 - 1	MANHOLE-WC-D	7	-0.0040	-7470A	PPB		25 Jun 2021 14:59:03	U	SMPL		
M2860-01 - 1	ASH	29	0.0014	-7470A	PPB		25 Jun 2021 15:01:18	U	SMPL		
PB137343BL - 1	PBW	12	-0.0028	-7470A	PPB		25 Jun 2021 15:03:33	U	SMPL		
PB137343BS - 1	LCSW	16043	3.9769	-7470A	PPB		25 Jun 2021 15:05:49	U	SMPL		
M2826-02 - 1	LS-1(LIQUID-BLUE)	-36	-0.0147	-7470A	PPB		25 Jun 2021 15:08:05	U	SMPL		
M2847-02 - 1	1928-29	78	0.0136	-7470A	PPB		25 Jun 2021 15:10:22	U	SMPL		
M2847-03 - 1	1970-WATER	-3	-0.0065	-7470A	PPB		25 Jun 2021 15:12:39	U	SMPL		
M2847-04 - 1	1962-1964	18	-0.0013	-7470A	PPB		25 Jun 2021 15:14:55	U	SMPL		
M2847-05 - 1	1966-1969	15	-0.0021	-7470A	PPB		25 Jun 2021 15:17:11	U	SMPL		
CCV70 - 1	CCV70	19860	4.9245	-7470A	PPB		25 Jun 2021 15:19:26	U	SMPL		
CCB70 - 1	CCB70	-114	-0.0341	-7470A	PPB		25 Jun 2021 15:21:42	U	SMPL		
M2847-06 - 1	1965	104	0.0200	-7470A	PPB		25 Jun 2021 15:23:57	U	SMPL		
M2848-02 - 1	OILY-WATER-DRUM	10	-0.0033	-7470A	PPB		25 Jun 2021 15:26:13	U	SMPL		
M2849-01 - 1	NWB-1613	11	-0.0031	-7470A	PPB		25 Jun 2021 15:28:28	U	SMPL		
M2849-01DUP - 1	NWB-1613DUP	30	0.0017	-7470A	PPB		25 Jun 2021 15:30:44	U	SMPL		
M2849-01MS - 1	NWB-1613MS	14922	3.6987	-7470A	PPB		25 Jun 2021 15:38:34	U	SMPL		
M2849-01MSD - 1	NWB-1613MSD	15179	3.7625	-7470A	PPB		25 Jun 2021 15:40:50	U	SMPL		
PB137344BL - 1	PBW	-91	-0.0284	-7470A	PPB		25 Jun 2021 15:43:06	U	SMPL		
PB137344BS - 1	LCSW	14711	3.6463	-7470A	PPB		25 Jun 2021 15:48:19	U	SMPL		
M2851-02 - 1	BACKFILL-ASHCROFT-REAR-07	169	0.0362	-7470A	PPB		25 Jun 2021 15:55:32	U	SMPL		
M2851-02DUP - 1	BACKFILL-ASHCROFT-REAR-07DUP	124	0.0250	-7470A	PPB		25 Jun 2021 15:57:47	U	SMPL		
CCV71 - 1	CCV71	19261	4.7758	-7470A	PPB		25 Jun 2021 16:00:02	U	SMPL		
CCB71 - 1	CCB71	-84	-0.0266	-7470A	PPB		25 Jun 2021 16:02:17	U	SMPL		
M2851-02MS - 1	BACKFILL-ASHCROFT-REAR-07MS	16026	3.9727	-7470A	PPB		25 Jun 2021 16:07:14	U	SMPL		
M2851-02MSD - 1	BACKFILL-ASHCROFT-REAR-07MSD	16263	4.0316	-7470A	PPB		25 Jun 2021 16:09:29	U	SMPL		
M2851-04 - 1	BACKFILL-ASHCROFT-REAR-08	318	0.0732	-7470A	PPB		25 Jun 2021 16:11:44	U	SMPL		
PB137345BL - 1	PBW	-6	-0.0073	-7470A	PPB		25 Jun 2021 16:14:00	U	SMPL		
PB137345BS - 1	LCSW	15977	3.9606	-7470A	PPB		25 Jun 2021 16:16:15	U	SMPL		
M2840-01 - 1	OUTFALL-TO-POND-1	13474	3.3392	-7470A	PPB		25 Jun 2021 16:18:31	U	SMPL		
M2840-01DUP - 1	OUTFALL-TO-POND-1DUP	13184	3.2672	-7470A	PPB		25 Jun 2021 16:20:48	U	SMPL		
M2840-01MS - 1	OUTFALL-TO-POND-1MS	27160	6.7368	-7470A	PPB		25 Jun 2021 16:23:04	U	SMPL		
M2840-01MSD - 1	OUTFALL-TO-POND-1MSD	26969	6.6894	-7470A	PPB		25 Jun 2021 16:25:21	U	SMPL		
M2840-02 - 1	POND-1	-55	-0.0194	-7470A	PPB		25 Jun 2021 16:27:38	U	SMPL		
CCV72 - 1	CCV72	19954	4.9479	-7470A	PPB		25 Jun 2021 16:29:55	U	SMPL		
CCB72 - 1	CCB72	-117	-0.0348	-7470A	PPB		25 Jun 2021 16:32:11	U	SMPL		
M2840-03 - 1	POND-2	20	-0.0008	-7470A	PPB		25 Jun 2021 16:34:26	U	SMPL		
M2840-04 - 1	OUTFALL-TO-POND-2	27	0.0009	-7470A	PPB		25 Jun 2021 16:36:42	U	SMPL		
PB137342TB - 1	PB137292TB	11	-0.0031	-7470A	PPB		25 Jun 2021 16:38:58	U	SMPL		
PB137343TB - 1	PB137338TB	5	-0.0045	-7470A	PPB		25 Jun 2021 16:41:14	U	SMPL		
PB137344TB - 1	PB137339TB	26	0.0007	-7470A	PPB		25 Jun 2021 16:43:30	U	SMPL		
M2812-02LX5 - 1		5	-0.0045	-7470A	PPB		25 Jun 2021 16:45:46	U	SMPL		
M2812-02A - 1		14652	3.6316	-7470A	PPB		25 Jun 2021 16:48:02	U	SMPL		
M2849-01LX5 - 1		-98	-0.0301	-7470A	PPB		25 Jun 2021 16:50:19	U	SMPL		
M2849-01A - 1		15899	3.9412	-7470A	PPB		25 Jun 2021 16:52:36	U	SMPL		
CCV73 - 1	CCV73	19127	4.7426	-7470A	PPB		25 Jun 2021 16:54:52	U	SMPL		
CCB73 - 1	CCB73	-141	-0.0408	-7470A	PPB		25 Jun 2021 16:57:08	U	SMPL		
M2851-02LX5 - 1		173	0.0372	-7470A	PPB		25 Jun 2021 16:59:24	U	SMPL		
M2851-02A - 1		14645	3.6299	-7470A	PPB		25 Jun 2021 17:01:40	U	SMPL		
M2840-01LX5 - 1		2739	0.6742	-7470A	PPB		25 Jun 2021 17:03:56	U	SMPL		
M2840-01A - 1		29346	7.2795	-7470A	PPB		25 Jun 2021 17:06:12	U	SMPL		
CCV74 - 1	CCV74	19312	4.7885	-7470A	PPB		25 Jun 2021 17:08:27	U	SMPL		
CCB74 - 1	CCB74	-146	-0.0420	-7470A	PPB		25 Jun 2021 17:10:44	U	SMPL		