


LB115134

7471B

INSTRUMENT ID: CV1

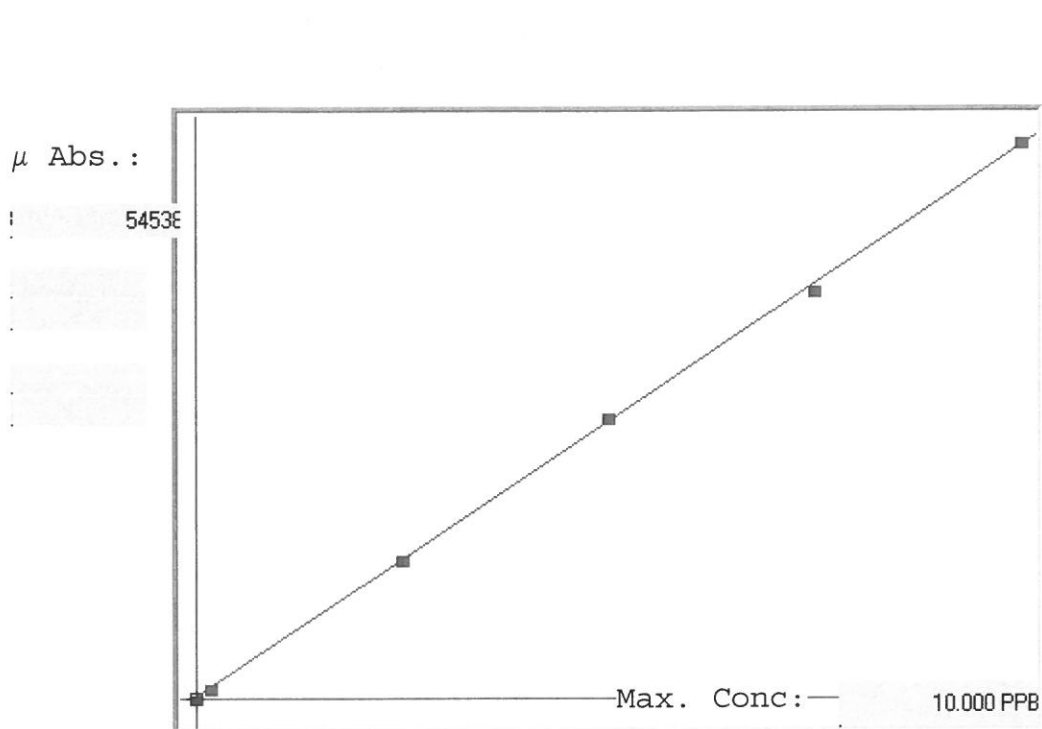

Linear

A= 0.0000e+000

B= 1.8443e-004

C= -1.6281e-002

Rho= 0.9998676

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.015	-0.015	5	0.000	5					-
0.2	0.200	0.192	-0.008	1129	0.0 %	1129					-4
2.5	2.500	2.523	0.023	13767	0.0 %	13767					1
5.0	5.000	5.075	0.075	27605	0.0 %	27605					2
7.5	7.500	7.384	-0.116	40126	0.0 %	40126					-2
10.0	10.000	10.042	0.042	54538	0.0 %	54538					0

LB115134 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 28 Jun 2021 14:29:56					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	5	-	0.0000	7471B	PPB	28 Jun 2021 15:14:50	S	Std
0.2 - 1	50.2	1129	-	0.2000	7471B	PPB	28 Jun 2021 15:17:07	S	Std
2.5 - 1	52.5	13767	-	2.5000	7471B	PPB	28 Jun 2021 15:19:23	S	Std
5.0 - 1	55	27605	-	5.0000	7471B	PPB	28 Jun 2021 15:21:40	S	Std
7.5 - 1	57.5	40126	-	7.5000	7471B	PPB	28 Jun 2021 15:23:57	S	Std
10.0 - 1	510	54538	-	10.0000	7471B	PPB	28 Jun 2021 15:26:12	S	Std
ICV79 - 1	ICV79	20817	3.8229	-	7471B	PPB	28 Jun 2021 15:28:59	U	SMPL
ICB79 - 1	ICB79	-124	-0.0392	-	7471B	PPB	28 Jun 2021 15:31:14	U	SMPL
CCV75 - 1	CCV75	27643	5.0818	-	7471B	PPB	28 Jun 2021 15:36:06	U	SMPL
CCB75 - 1	CCB75	-137	-0.0415	-	7471B	PPB	28 Jun 2021 15:38:20	U	SMPL
CRA - 1	CRA	1111	0.1886	-	7471B	PPB	28 Jun 2021 15:40:36	U	SMPL
HighStd - 1	HighStd	54531	10.0406	-	7471B	PPB	28 Jun 2021 15:42:51	U	SMPL
ChkStd - 1	ChkStd	38150	7.0196	-	7471B	PPB	28 Jun 2021 15:45:06	U	SMPL
PB137398BL - 1	PBS	4	-0.0155	-	7471B	PPB	28 Jun 2021 15:49:56	U	SMPL
PB137398BS - 1	LCSS	18905	3.4703	-	7471B	PPB	28 Jun 2021 15:52:12	U	SMPL
M2864-02 - 1	VNJ-206	1831	0.3214	-	7471B	PPB	28 Jun 2021 15:59:32	U	SMPL
M2864-02DUP - 1	VNJ-206DUP	1730	0.3028	-	7471B	PPB	28 Jun 2021 16:01:48	U	SMPL
M2864-02MS - 1	VNJ-206MS	22475	4.1287	-	7471B	PPB	28 Jun 2021 16:04:05	U	SMPL
M2864-02MSD - 1	VNJ-206MSD	23416	4.3022	-	7471B	PPB	28 Jun 2021 16:06:22	U	SMPL
M2864-04 - 1	12002	23176	4.2580	-	7471B	PPB	28 Jun 2021 16:08:37	U	SMPL
CCV76 - 1	CCV76	27405	5.0379	-	7471B	PPB	28 Jun 2021 16:10:52	U	SMPL
CCB76 - 1	CCB76	-149	-0.0438	-	7471B	PPB	28 Jun 2021 16:13:08	U	SMPL
M2865-01 - 1	OR-01-062521	5893	1.0705	-	7471B	PPB	28 Jun 2021 16:15:23	U	SMPL
M2866-01 - 1	124055	2917	0.5217	-	7471B	PPB	28 Jun 2021 16:17:39	U	SMPL
M2866-03 - 1	124030	3655	0.6578	-	7471B	PPB	28 Jun 2021 16:19:55	U	SMPL
M2866-05 - 1	124019	4050	0.7306	-	7471B	PPB	28 Jun 2021 16:22:10	U	SMPL
M2866-07 - 1	124042	2500	0.4448	-	7471B	PPB	28 Jun 2021 16:24:26	U	SMPL
M2867-01 - 1	OILY-SOCK-DRUM	107	0.0035	-	7471B	PPB	28 Jun 2021 16:26:42	U	SMPL
M2867-03 - 1	OILY-STONE-DRUM	34	-0.0100	-	7471B	PPB	28 Jun 2021 16:28:59	U	SMPL
M2864-02LX5 - 1		342	0.0468	-	7471B	PPB	28 Jun 2021 16:31:15	U	SMPL
M2864-02A - 1		24700	4.5390	-	7471B	PPB	28 Jun 2021 16:33:33	U	SMPL
CCV77 - 1	CCV77	26769	4.9206	-	7471B	PPB	28 Jun 2021 16:35:48	U	SMPL
CCB77 - 1	CCB77	-127	-0.0397	-	7471B	PPB	28 Jun 2021 16:38:03	U	SMPL