


LB115148

7470A

INSTRUMENT ID: CV1

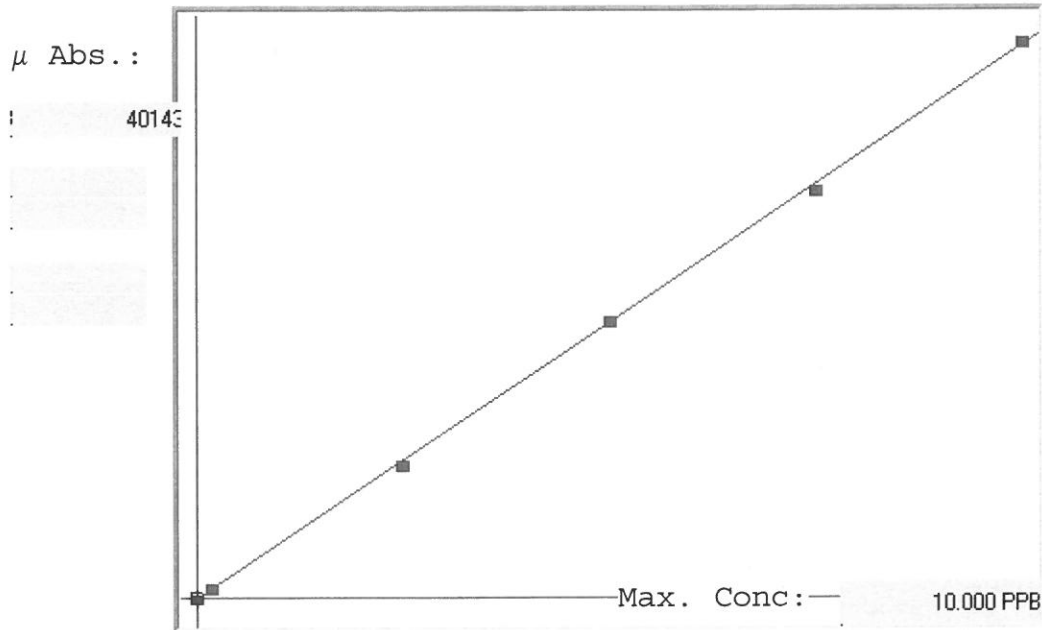

Linear

A= 0.0000e+000

B= 2.4996e-004

C= 2.8635e-002

Rho= 0.9998907

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.036	0.036	30	0.000	30					1
0.2	0.200	0.214	0.014	742	0.0 %	742					7
2.5	2.500	2.444	-0.056	9661	0.0 %	9661					-2
5.0	5.000	5.033	0.033	20022	0.0 %	20022					1
7.5	7.500	7.410	-0.090	29530	0.0 %	29530					-1
10.0	10.000	10.063	0.063	40143	0.0 %	40143					1

Method: 7470A		Operator: Admin		Date of Analysis: 29 Jun 2021 10:46:44					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	30	-	0.0000	7470A	PPB	29 Jun 2021	10:53:05	S Std
0.2 - 1	51.2	742	-	0.2000	7470A	PPB	29 Jun 2021	10:55:23	S Std
2.5 - 1	52.5	9661	-	2.5000	7470A	PPB	29 Jun 2021	10:57:39	S Std
5.0 - 1	55	20022	-	5.0000	7470A	PPB	29 Jun 2021	10:59:56	S Std
7.5 - 1	57.7	29530	-	7.5000	7470A	PPB	29 Jun 2021	11:02:12	S Std
10.0 - 1	610	40143	-	10.0000	7470A	PPB	29 Jun 2021	11:09:48	S Std
ICV80 - 1	ICV80	15295	3.8518	-	7470A	PPB	29 Jun 2021	11:14:27	U SMPL
ICB80 - 1	ICB80	-82	0.0081	-	7470A	PPB	29 Jun 2021	11:16:41	U SMPL
CCV78 - 1	CCV78	20588	5.1749	-	7470A	PPB	29 Jun 2021	11:18:56	U SMPL
CCB78 - 1	CCB78	-98	0.0041	-	7470A	PPB	29 Jun 2021	11:21:11	U SMPL
CRA - 1	CRA	761	0.2189	-	7470A	PPB	29 Jun 2021	11:23:26	U SMPL
HighStd - 1	HighStd	40327	10.1089	-	7470A	PPB	29 Jun 2021	11:25:41	U SMPL
ChkStd - 1	ChkStd	28372	7.1206	-	7470A	PPB	29 Jun 2021	11:27:56	U SMPL
PB137385BL - 1	PBW	-141	-0.0066	-	7470A	PPB	29 Jun 2021	11:30:12	U SMPL
PB137385BS - 1	LCSW	14848	3.7401	-	7470A	PPB	29 Jun 2021	11:32:29	U SMPL
M2856-21 - 1	SB-01-COMP	-84	0.0076	-	7470A	PPB	29 Jun 2021	11:34:45	U SMPL
M2856-21DUP - 1	SB-01-COMPDUP	4	0.0296	-	7470A	PPB	29 Jun 2021	11:37:02	U SMPL
M2856-21MS - 1	SB-01-COMPMS	15147	3.8148	-	7470A	PPB	29 Jun 2021	11:39:18	U SMPL
M2856-21MSD - 1	SB-01-COMPMSD	16369	4.1203	-	7470A	PPB	29 Jun 2021	11:41:36	U SMPL
M2856-22 - 1	SB-02-COMP	-96	0.0046	-	7470A	PPB	29 Jun 2021	11:43:51	U SMPL
CCV79 - 1	CCV79	20407	5.1296	-	7470A	PPB	29 Jun 2021	11:46:07	U SMPL
CCB79 - 1	CCB79	-103	0.0029	-	7470A	PPB	29 Jun 2021	11:48:22	U SMPL
M2856-23 - 1	SB-03-COMP	3	0.0294	-	7470A	PPB	29 Jun 2021	11:50:37	U SMPL
M2856-24 - 1	SB-04-COMP	11	0.0314	-	7470A	PPB	29 Jun 2021	11:52:52	U SMPL
M2856-25 - 1	SB-05-COMP	17	0.0329	-	7470A	PPB	29 Jun 2021	11:55:08	U SMPL
M2856-26 - 1	SB-06-COMP	22	0.0341	-	7470A	PPB	29 Jun 2021	11:57:23	U SMPL
M2856-27 - 1	SB-07-COMP	34	0.0371	-	7470A	PPB	29 Jun 2021	11:59:38	U SMPL
M2856-28 - 1	SB-08-COMP	28	0.0356	-	7470A	PPB	29 Jun 2021	12:01:55	U SMPL
M2856-29 - 1	SB-09-COMP	36	0.0376	-	7470A	PPB	29 Jun 2021	12:04:11	U SMPL
M2856-30 - 1	SB-10-COMP	47	0.0404	-	7470A	PPB	29 Jun 2021	12:06:29	U SMPL
M2857-17 - 1	SB-11-COMP	25	0.0349	-	7470A	PPB	29 Jun 2021	12:08:45	U SMPL
M2857-18 - 1	SB-12-COMP	29	0.0359	-	7470A	PPB	29 Jun 2021	12:11:00	U SMPL
CCV80 - 1	CCV80	20408	5.1299	-	7470A	PPB	29 Jun 2021	12:13:15	U SMPL
CCB80 - 1	CCB80	-103	0.0029	-	7470A	PPB	29 Jun 2021	12:15:31	U SMPL
M2857-19 - 1	SB-13-COMP	3	0.0294	-	7470A	PPB	29 Jun 2021	12:17:46	U SMPL
M2857-20 - 1	SB-14-COMP	11	0.0314	-	7470A	PPB	29 Jun 2021	12:20:01	U SMPL
M2857-21 - 1	SB-15-COMP	13	0.0319	-	7470A	PPB	29 Jun 2021	12:22:16	U SMPL
M2857-22 - 1	SB-16-COMP	7	0.0304	-	7470A	PPB	29 Jun 2021	12:24:32	U SMPL
M2857-23 - 1	SB-17-COMP	17	0.0329	-	7470A	PPB	29 Jun 2021	12:26:48	U SMPL
M2857-24 - 1	SB-18-COMP	21	0.0339	-	7470A	PPB	29 Jun 2021	12:29:04	U SMPL
PB137386BL - 1	PBW	19	0.0334	-	7470A	PPB	29 Jun 2021	12:31:20	U SMPL
PB137386BS - 1	LCSW	14224	3.5841	-	7470A	PPB	29 Jun 2021	12:33:37	U SMPL
M2866-02 - 1	124055	-68	0.0116	-	7470A	PPB	29 Jun 2021	12:35:54	U SMPL
M2866-02DUP - 1	124055DUP	3	0.0294	-	7470A	PPB	29 Jun 2021	12:38:09	U SMPL
CCV81 - 1	CCV81	20504	5.1539	-	7470A	PPB	29 Jun 2021	12:40:25	U SMPL
CCB81 - 1	CCB81	-106	0.0021	-	7470A	PPB	29 Jun 2021	12:42:40	U SMPL
M2866-02MS - 1	124055MS	14596	3.6771	-	7470A	PPB	29 Jun 2021	12:44:55	U SMPL
M2866-02MSD - 1	124055MSD	14608	3.6801	-	7470A	PPB	29 Jun 2021	12:47:11	U SMPL
M2866-04 - 1	124030	-94	0.0051	-	7470A	PPB	29 Jun 2021	12:49:26	U SMPL
M2866-06 - 1	124019	8	0.0306	-	7470A	PPB	29 Jun 2021	12:51:41	U SMPL
M2866-08 - 1	124042	12	0.0316	-	7470A	PPB	29 Jun 2021	12:53:57	U SMPL
M2868-01 - 1	OILY-DEBRIS-TRE-1169	17	0.0329	-	7470A	PPB	29 Jun 2021	12:56:14	U SMPL
PB137387BL - 1	PBW	25	0.0349	-	7470A	PPB	29 Jun 2021	12:58:30	U SMPL
PB137387BS - 1	LCSW	15317	3.8573	-	7470A	PPB	29 Jun 2021	13:00:47	U SMPL
M2868-03 - 1	WASTE-WATER-TRE-1202	-62	0.0131	-	7470A	PPB	29 Jun 2021	13:03:04	U SMPL
M2868-03DUP - 1	WASTE-WATER-TRE-1202DUP	11	0.0314	-	7470A	PPB	29 Jun 2021	13:05:19	U SMPL
CCV82 - 1	CCV82	20597	5.1771	-	7470A	PPB	29 Jun 2021	13:07:35	U SMPL
CCB82 - 1	CCB82	-104	0.0026	-	7470A	PPB	29 Jun 2021	13:09:50	U SMPL
M2868-03MS - 1	WASTE-WATER-TRE-1202MS	15259	3.8428	-	7470A	PPB	29 Jun 2021	13:12:05	U SMPL
M2868-03MSD - 1	WASTE-WATER-TRE-1202MSD	14799	3.7278	-	7470A	PPB	29 Jun 2021	13:14:21	U SMPL
PB137386TB - 1	PB137351TB	-86	0.0071	-	7470A	PPB	29 Jun 2021	13:16:37	U SMPL
PB137385TB - 1	PB137362TB	-12	0.0256	-	7470A	PPB	29 Jun 2021	13:18:52	U SMPL
PB137387TB - 1	PB137364TB	22	0.0341	-	7470A	PPB	29 Jun 2021	13:21:08	U SMPL
CCV83 - 1	CCV83	20379	5.1226	-	7470A	PPB	29 Jun 2021	13:23:24	U SMPL
CCB83 - 1	CCB83	-94	0.0051	-	7470A	PPB	29 Jun 2021	13:25:40	U SMPL
M2856-21LX5 - 1		18	0.0331	-	7470A	PPB	29 Jun 2021	13:27:56	U SMPL
M2856-21A - 1		15788	3.9750	-	7470A	PPB	29 Jun 2021	13:30:13	U SMPL
M2866-02LX5 - 1		-73	0.0104	-	7470A	PPB	29 Jun 2021	13:32:29	U SMPL
M2866-02A - 1		15244	3.8391	-	7470A	PPB	29 Jun 2021	13:34:45	U SMPL
M2868-03LX5 - 1		-69	0.0114	-	7470A	PPB	29 Jun 2021	13:37:00	U SMPL
M2868-03A - 1		15252	3.8411	-	7470A	PPB	29 Jun 2021	13:39:16	U SMPL
CCV84 - 1	CCV84	20443	5.1386	-	7470A	PPB	29 Jun 2021	13:41:32	U SMPL
CCB84 - 1	CCB84	-112	0.0006	-	7470A	PPB	29 Jun 2021	13:43:48	U SMPL