


LB 115160

7470A

INSTRUMENT ID: CV1

 μ Abs.:

39987

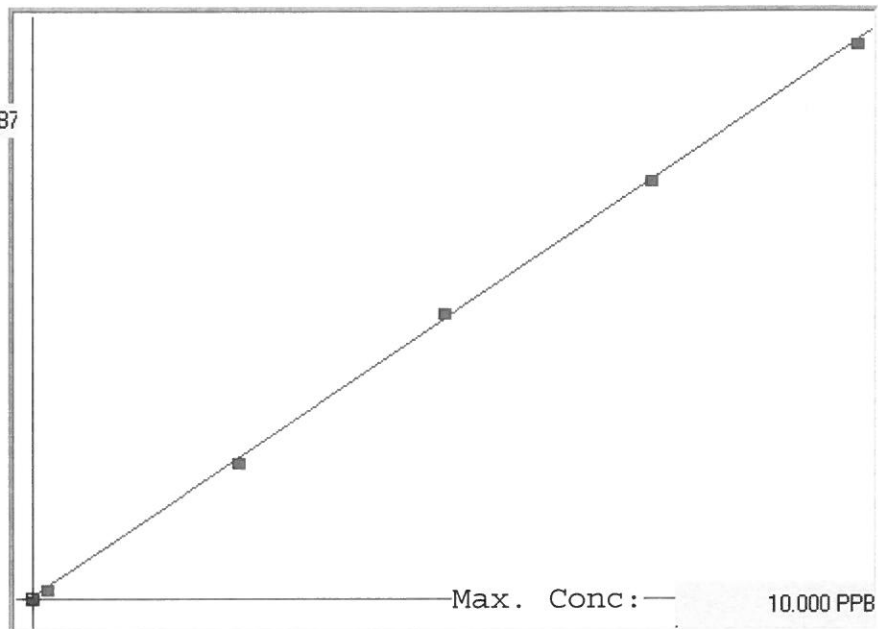

A= 0.0000e+000

B= 2.4918e-004

C= -2.1377e-002

Rho= 0.9998672

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Y/D
0.0	0.000	0.001	0.001	91	0.000	91					1
0.2	0.200	0.184	-0.016	826	0.0 %	826					-8
2.5	2.500	2.437	-0.063	9867	0.0 %	9867					-3
5.0	5.000	5.118	0.118	20626	0.0 %	20626					2
7.5	7.500	7.516	0.016	30248	0.0 %	30248					0
10.0	10.000	9.943	-0.057	39987	0.0 %	39987					-1

LB115160 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 30 Jun 2021 11:33:22						Date	Type	Type
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units						
0.0 - 1	50	91	-	0.0000	7470A	PPB				30 Jun 2021 11:36:04	S	Std
0.2 - 1	502	826	-	0.2000	7470A	PPB				30 Jun 2021 11:38:21	S	Std
2.5 - 1	52.5	9867	-	2.5000	7470A	PPB				30 Jun 2021 11:40:38	S	Std
5.0 - 1	55	20626	-	5.0000	7470A	PPB				30 Jun 2021 11:42:54	S	Std
7.5 - 1	57.5	30248	-	7.5000	7470A	PPB				30 Jun 2021 11:45:11	S	Std
10.0 - 1	518	39987	-	10.0000	7470A	PPB				30 Jun 2021 11:50:00	S	Std
ICV82 - 1	ICV82	15219	3.7709	-	7470A	PPB				30 Jun 2021 11:52:45	U	SMPL
ICB82 - 1	ICB82	-93	-0.0446	-	7470A	PPB				30 Jun 2021 11:54:59	U	SMPL
CCV89 - 1	CCV89	19722	4.8930	-	7470A	PPB				30 Jun 2021 11:57:14	U	SMPL
CCB89 - 1	CCB89	-88	-0.0433	-	7470A	PPB				30 Jun 2021 11:59:29	U	SMPL
CRA - 1	CRA	765	0.1692	-	7470A	PPB				30 Jun 2021 12:01:43	U	SMPL
HighStd - 1	HighStd	40282	10.0162	-	7470A	PPB				30 Jun 2021 12:03:58	U	SMPL
ChkStd - 1	ChkStd	26150	6.4948	-	7470A	PPB				30 Jun 2021 12:06:14	U	SMPL
PB137422BL - 1	PBW	-94	-0.0448	-	7470A	PPB				30 Jun 2021 12:08:30	U	SMPL
PB137422BS - 1	LCSW	13956	3.4562	-	7470A	PPB				30 Jun 2021 12:10:46	U	SMPL
M2882-03 - 1	DRIP-COMP-AUD-1121-1122	28	-0.0144	-	7470A	PPB				30 Jun 2021 12:13:03	U	SMPL
M2882-05 - 1	SEALPOT-AUD-1123	245	0.0397	-	7470A	PPB				30 Jun 2021 12:20:10	U	SMPL
M2882-05DUP - 1	SEALPOT-AUD-1123DUP	187	0.0252	-	7470A	PPB				30 Jun 2021 12:22:26	U	SMPL
M2882-05MS - 1	SEALPOT-AUD-1123MS	13806	3.4189	-	7470A	PPB				30 Jun 2021 12:24:43	U	SMPL
M2882-05MSD - 1	SEALPOT-AUD-1123MSD	13251	3.2806	-	7470A	PPB				30 Jun 2021 12:29:39	U	SMPL
CCV90 - 1	CCV90	19571	4.8554	-	7470A	PPB				30 Jun 2021 12:31:54	U	SMPL
CCB90 - 1	CCB90	-65	-0.0376	-	7470A	PPB				30 Jun 2021 12:34:08	U	SMPL
M2882-07 - 1	AUD-1126	93	0.0018	-	7470A	PPB				30 Jun 2021 12:36:24	U	SMPL
PB137423BL - 1	PBW	111	0.0063	-	7470A	PPB				30 Jun 2021 12:38:39	U	SMPL
PB137423BS - 1	LCSW	15863	3.9314	-	7470A	PPB				30 Jun 2021 12:44:30	U	SMPL
M2889-06 - 1	TW-1	247	0.0402	-	7470A	PPB				30 Jun 2021 12:46:45	U	SMPL
M2889-06DUP - 1	TW-1DUP	311	0.0561	-	7470A	PPB				30 Jun 2021 12:49:01	U	SMPL
M2889-06MS - 1	TW-1MS	13955	3.4560	-	7470A	PPB				30 Jun 2021 12:51:17	U	SMPL
M2889-06MSD - 1	TW-1MSD	14134	3.5006	-	7470A	PPB				30 Jun 2021 12:53:33	U	SMPL
M2889-07 - 1	TW-2	66	-0.0049	-	7470A	PPB				30 Jun 2021 12:55:50	U	SMPL
M2889-08 - 1	TW-3	118	0.0080	-	7470A	PPB				30 Jun 2021 12:58:06	U	SMPL
CCV91 - 1	CCV91	19672	4.8806	-	7470A	PPB				30 Jun 2021 13:00:22	U	SMPL
CCB91 - 1	CCB91	-51	-0.0341	-	7470A	PPB				30 Jun 2021 13:02:37	U	SMPL
PB137422TB - 1	PB137405TB	79	-0.0017	-	7470A	PPB				30 Jun 2021 13:04:52	U	SMPL
M2882-05LX5 - 1		289	0.0506	-	7470A	PPB				30 Jun 2021 13:07:08	U	SMPL
M2882-05A - 1		15779	3.9105	-	7470A	PPB				30 Jun 2021 13:09:23	U	SMPL
M2889-06LX5 - 1		51	-0.0087	-	7470A	PPB				30 Jun 2021 13:11:39	U	SMPL
M2889-06A - 1		15596	3.8649	-	7470A	PPB				30 Jun 2021 13:13:54	U	SMPL
CCV92 - 1	CCV92	19410	4.8153	-	7470A	PPB				30 Jun 2021 13:16:09	U	SMPL
CCB92 - 1	CCB92	-83	-0.0421	-	7470A	PPB				30 Jun 2021 13:18:26	U	SMPL