

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : MA

Instrument ID : Konelab

7/1/2021 15:09

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.156	0.0	0.070	
ICB1	0.648	0.0	0.001	
CCV1	244.981	0.0	0.175	
CCB1	0.344	0.0	0.001	
PB137413BL	0.492	0.0	0.001	
PB137413BS	97.911	0.0	0.070	
LOWPB137413	9.955	0.0	0.008	
HIGHPB137413	478.934	0.0	0.341	
M2864-01	1.798	0.0	0.002	
M2864-01DUP	1.898	0.0	0.002	
M2864-01MS	45.342	0.0	0.033	
M2864-01MSD	45.412	0.0	0.033	
M2864-04	1.409	0.0	0.002	
M2899-01	1.029	0.0	0.001	
CCV2	246.647	0.0	0.176	
CCB2	0.618	0.0	0.001	

N	16
Mean	79.723
SD	134.6564
CV%	168.90

limit
- 99.4. (90-110)
- 96.4.

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

7/1/2021 14:26

Reviewed by : AY Instrument ID : Konelab


Test Total CN

Accepted 7/1/2021 14:26

Factor 1406
Bias 0.001

Coeff. of det. 0.999852

Errors

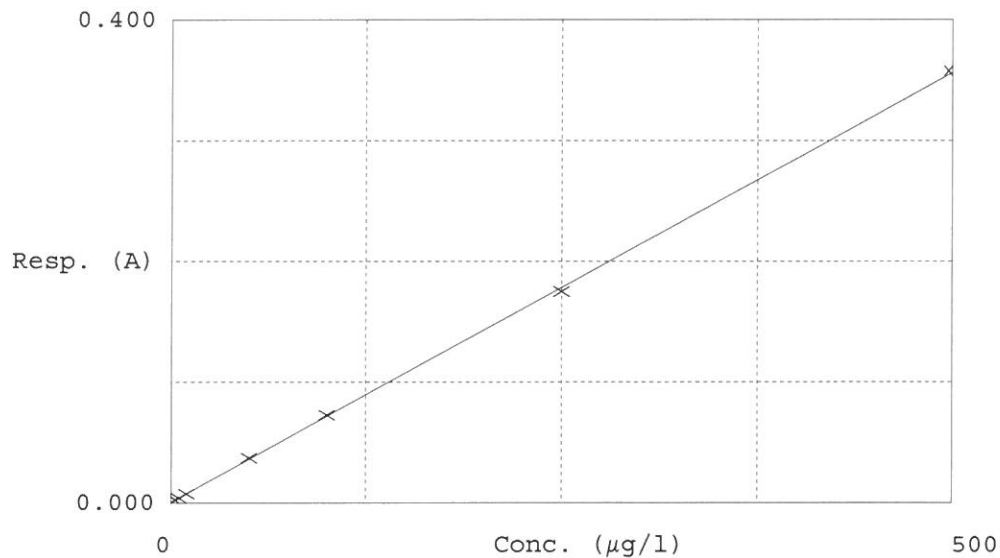

	Calibrator	Response	Calc. con.	Conc.	Relative Errors
1	0.0PPBCN	0.001	0.5681	0.0000	
2	5.0PPBCN	0.004	4.9220	5.0000	-1.5
3	10PPBCN	0.008	9.7358	10.0000	-2.6
4	50PPBCN	0.037	51.2859	50.0000	-2.6
5	100PPBCN	0.073	101.2443	100.0000	1.2
6	250PPBCN	0.175	245.2306	250.0000	-1.9
7	500PPBCN	0.358	502.0133	500.0000	0.4

AY
7/1/21

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 01 13:30:33 2021

Thu Jul 01 15:06:56 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.5681	µg/l	7/1/2021 14:26:19	
5.OPPBCN	A	Total CN	P	4.922	µg/l	7/1/2021 14:26:20	
10PPBCN	A	Total CN	P	9.7358	µg/l	7/1/2021 14:26:21	
50PPBCN	A	Total CN	P	51.2859	µg/l	7/1/2021 14:26:22	
100PPBCN	A	Total CN	P	101.2443	µg/l	7/1/2021 14:26:23	
250PPBCN	A	Total CN	P	245.2306	µg/l	7/1/2021 14:26:24	
500PPBCN	A	Total CN	P	502.0133	µg/l	7/1/2021 14:26:25	
ICV1	S	Total CN	P	98.1561	µg/l	7/1/2021 14:56:33	
ICB1	S	Total CN	P	0.648	µg/l	7/1/2021 14:56:36	
CCV1	S	Total CN	P	244.9813	µg/l	7/1/2021 14:56:37	
CCB1	S	Total CN	P	0.3442	µg/l	7/1/2021 14:56:40	
PB137413BL	S	Total CN	P	0.4923	µg/l	7/1/2021 14:56:41	
PB137413BS	S	Total CN	P	97.9106	µg/l	7/1/2021 14:56:42	
LOWPB137413	S	Total CN	P	9.9547	µg/l	7/1/2021 14:56:43	
HIGHPB137413	S	Total CN	P	478.9344	µg/l	7/1/2021 15:04:08	
M2864-01	S	Total CN	P	1.7982	µg/l	7/1/2021 15:04:09	
M2864-01DUP	S	Total CN	P	1.898	µg/l	7/1/2021 15:04:10	
M2864-01MS	S	Total CN	P	45.3424	µg/l	7/1/2021 15:04:13	
M2864-01MSD	S	Total CN	P	45.4124	µg/l	7/1/2021 15:04:14	
M2864-04	S	Total CN	P	1.4092	µg/l	7/1/2021 15:04:15	
M2899-01	S	Total CN	P	1.0289	µg/l	7/1/2021 15:04:16	
CCV2	S	Total CN	P	246.6474	µg/l	7/1/2021 15:04:17	
CCB2	S	Total CN	P	0.6175	µg/l	7/1/2021 15:04:18	