


LB115176

7470A

INSTRUMENT ID: CV1

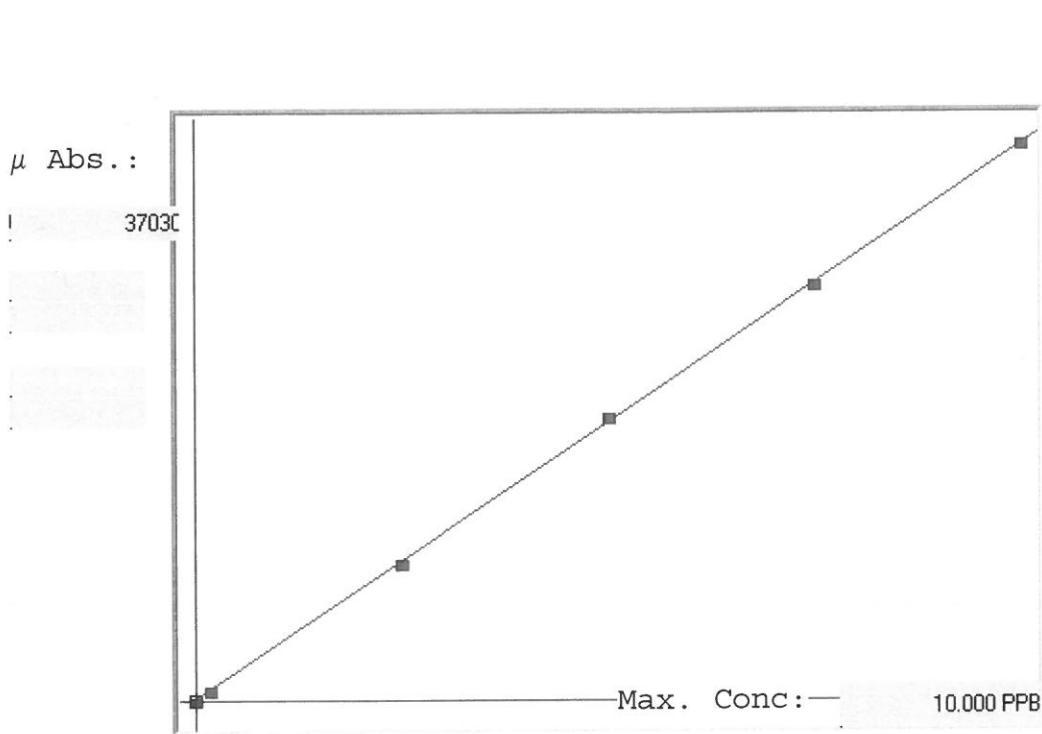

Linear

A= 0.0000e+000

B= 2.7024e-004

C= -1.4792e-002

Rho= 0.9999306

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/d)
0.0	0.000	0.015	0.015	112	0.000	112					-
0.2	0.200	0.190	-0.010	758	0.0 %	758					-5
2.5	2.500	2.447	-0.053	9110	0.0 %	9110					-2
5.0	5.000	5.085	0.085	18872	0.0 %	18872					2
7.5	7.500	7.470	-0.030	27698	0.0 %	27698					0
10.0	10.000	9.992	-0.008	37030	0.0 %	37030					0

LB115176 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Jul 2021 10:35:19

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	112	-	0.0000	7470A	PPB	01 Jul 2021 10:44:41	S	Std
0.2 - 1	50.2	758	-	0.2000	7470A	PPB	01 Jul 2021 10:46:58	S	Std
2.5 - 1	52.5	9110	-	2.5000	7470A	PPB	01 Jul 2021 10:49:15	S	Std
5.0 - 1	53	18872	-	5.0000	7470A	PPB	01 Jul 2021 10:51:31	S	Std
7.5 - 1	57.5	27698	-	7.5000	7470A	PPB	01 Jul 2021 10:53:48	S	Std
10.0 - 1	57.5	37030	-	10.0000	7470A	PPB	01 Jul 2021 10:56:03	S	Std
ICV85 - 1	ICV85	15132	4.0744	-	7470A	PPB	01 Jul 2021 10:58:42	U	SMPL
ICB85 - 1	ICB85	49	-0.0016	-	7470A	PPB	01 Jul 2021 11:00:56	U	SMPL
CCV01 - 1	CCV01	18112	4.8797	-	7470A	PPB	01 Jul 2021 11:03:11	U	SMPL
CCB01 - 1	CCB01	45	-0.0026	-	7470A	PPB	01 Jul 2021 11:05:26	U	SMPL
CRA - 1	CRA	755	0.1892	-	7470A	PPB	01 Jul 2021 11:07:41	U	SMPL
HighStd - 1	HighStd	36912	9.9602	-	7470A	PPB	01 Jul 2021 11:09:55	U	SMPL
ChkStd - 1	ChkStd	26332	7.1011	-	7470A	PPB	01 Jul 2021 11:12:10	U	SMPL
PB137451BL - 1	PBW	-37	-0.0248	-	7470A	PPB	01 Jul 2021 11:14:27	U	SMPL
PB137451BS - 1	LCSW	15277	4.1136	-	7470A	PPB	01 Jul 2021 11:19:22	U	SMPL
M2896-02 - 1	FS-01	47	-0.0021	-	7470A	PPB	01 Jul 2021 11:21:38	U	SMPL
M2896-04 - 1	FS-02	148	0.0252	-	7470A	PPB	01 Jul 2021 11:23:54	U	SMPL
M2896-06 - 1	FS-03	150	0.0257	-	7470A	PPB	01 Jul 2021 11:26:11	U	SMPL
M2896-08 - 1	FS-04	87	0.0087	-	7470A	PPB	01 Jul 2021 11:28:28	U	SMPL
M2896-08DUP - 1	FS-04DUP	91	0.0098	-	7470A	PPB	01 Jul 2021 11:30:43	U	SMPL
CCV02 - 1	CCV02	18393	4.9557	-	7470A	PPB	01 Jul 2021 11:32:58	U	SMPL
CCB02 - 1	CCB02	52	-0.0007	-	7470A	PPB	01 Jul 2021 11:35:14	U	SMPL
M2896-08MS - 1	FS-04MS	14630	3.9388	-	7470A	PPB	01 Jul 2021 11:37:29	U	SMPL
M2896-08MSD - 1	FS-04MSD	14527	3.9109	-	7470A	PPB	01 Jul 2021 11:39:43	U	SMPL
PB137451TB - 1	PB137428TB	44	-0.0029	-	7470A	PPB	01 Jul 2021 11:41:58	U	SMPL
M2896-08LX5 - 1		142	0.0236	-	7470A	PPB	01 Jul 2021 11:44:14	U	SMPL
M2896-08A - 1		14545	3.9158	-	7470A	PPB	01 Jul 2021 11:46:30	U	SMPL
CCV03 - 1	CCV03	18018	4.8543	-	7470A	PPB	01 Jul 2021 11:48:46	U	SMPL
CCB03 - 1	CCB03	72	0.0047	-	7470A	PPB	01 Jul 2021 11:51:02	U	SMPL