

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AK Instrument ID : Konelab

7/1/2021 15:55

Test: ~~Total~~ CN *Native* *mu*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.605	0.0	0.070	
ICB1	0.262	0.0	0.001	
CCV1	248.547	0.0	0.177	
CCB1	0.581	0.0	0.001	
PB137460BL	0.694	0.0	0.001	
M2908-02	0.462	0.0	0.001	
M2908-02DUP	0.424	0.0	0.001	
PB137449BL	0.398	0.0	0.001	
M2894-02	0.701	0.0	0.001	
M2894-02DUP	0.692	0.0	0.001	
M2900-01	0.728	0.0	0.001	
M2908-01	0.613	0.0	0.001	
M2913-02	0.763	0.0	0.001	
M2913-04	0.459	0.0	0.001	
CCV2	246.910	0.0	0.176	
CCB2	0.689	0.0	0.001	
M2913-06	0.547	0.0	0.001	
M2913-08	0.119	0.0	0.001	
M2913-10	-0.222	0.0	0.000	
M2913-12	-0.205	0.0	0.000	
M2913-14	0.170	0.0	0.001	
M2913-16	0.147	0.0	0.001	
M2913-18	0.136	0.0	0.001	
CCV3	257.169	0.0	0.183	
CCB3	0.427	0.0	0.001	

N	25
Mean	34.353
SD	83.8911
CV%	244.21

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AI

Instrument ID : Konelab

7/1/2021 14:26


Test Total CN

Accepted 7/1/2021 14:26

Factor 1406
Bias 0.001

Coeff. of det. 0.999852

Errors

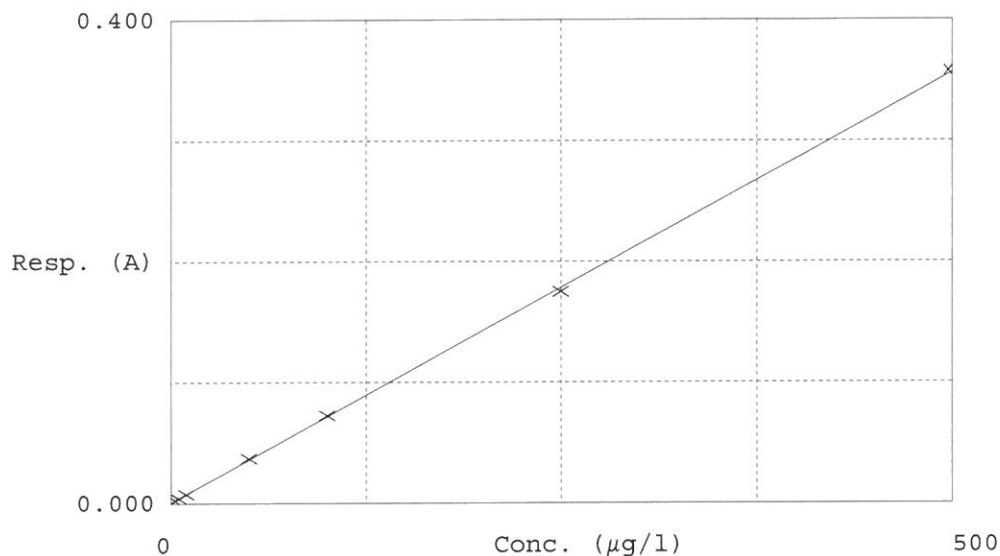

	Calibrator	Response	Calc. con.	Conc.	Relative Errors
1	0.0PPBCN	0.001	0.5681	0.0000	
2	5.0PPBCN	0.004	4.9220	5.0000	-1.5
3	10PPBCN	0.008	9.7358	10.0000	-2.6
4	50PPBCN	0.037	51.2859	50.0000	-2.6
5	100PPBCN	0.073	101.2443	100.0000	1.2
6	250PPBCN	0.175	245.2306	250.0000	-1.9
7	500PPBCN	0.358	502.0133	500.0000	0.4

AI
7/1/21

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 01 15:39:49 2021

Thu Jul 01 15:54:46 2021

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.5681	µg/l	7/1/2021 14:26:19	
5.OPPBCN	A	Reactive CN	P	4.922	µg/l	7/1/2021 14:26:20	
10PPBCN	A	Reactive CN	P	9.7358	µg/l	7/1/2021 14:26:21	
50PPBCN	A	Reactive CN	P	51.2859	µg/l	7/1/2021 14:26:22	
100PPBCN	A	Reactive CN	P	101.2443	µg/l	7/1/2021 14:26:23	
250PPBCN	A	Reactive CN	P	245.2306	µg/l	7/1/2021 14:26:24	
500PPBCN	A	Reactive CN	P	502.0133	µg/l	7/1/2021 14:26:25	
ICV1	S	Reactive CN	P	97.6053	µg/l	7/1/2021 15:39:49	
ICB1	S	Reactive CN	P	0.2619	µg/l	7/1/2021 15:39:51	
CCV1	S	Reactive CN	P	248.5467	µg/l	7/1/2021 15:39:53	
CCB1	S	Reactive CN	P	0.5809	µg/l	7/1/2021 15:39:56	
PB137460BL	S	Reactive CN	P	0.6942	µg/l	7/1/2021 15:39:57	
M2908-02	S	Reactive CN	P	0.4621	µg/l	7/1/2021 15:39:58	
M2908-02DUP	S	Reactive CN	P	0.4237	µg/l	7/1/2021 15:39:59	
PB137449BL	S	Reactive CN	P	0.3983	µg/l	7/1/2021 15:47:24	
M2894-02	S	Reactive CN	P	0.7008	µg/l	7/1/2021 15:47:25	
M2894-02DUP	S	Reactive CN	P	0.6919	µg/l	7/1/2021 15:47:26	
M2900-01	S	Reactive CN	P	0.7278	µg/l	7/1/2021 15:47:27	
M2908-01	S	Reactive CN	P	0.6128	µg/l	7/1/2021 15:47:28	
M2913-02	S	Reactive CN	P	0.7634	µg/l	7/1/2021 15:47:29	
M2913-04	S	Reactive CN	P	0.4585	µg/l	7/1/2021 15:47:30	
CCV2	S	Reactive CN	P	246.9095	µg/l	7/1/2021 15:47:31	
CCB2	S	Reactive CN	P	0.6887	µg/l	7/1/2021 15:47:32	
M2913-06	S	Reactive CN	P	0.5466	µg/l	7/1/2021 15:47:33	
M2913-08	S	Reactive CN	P	0.1186	µg/l	7/1/2021 15:47:34	
M2913-10	S	Reactive CN	P	-0.2218	µg/l	7/1/2021 15:52:11	
M2913-12	S	Reactive CN	P	-0.2047	µg/l	7/1/2021 15:52:12	
M2913-14	S	Reactive CN	P	0.1703	µg/l	7/1/2021 15:52:13	
M2913-16	S	Reactive CN	P	0.1474	µg/l	7/1/2021 15:52:14	
M2913-18	S	Reactive CN	P	0.1364	µg/l	7/1/2021 15:52:15	
CCV3	S	Reactive CN	P	257.1688	µg/l	7/1/2021 15:54:45	
CCB3	S	Reactive CN	P	0.4271	µg/l	7/1/2021 15:54:46	