


LB115192

7470A

INSTRUMENT ID: CV1

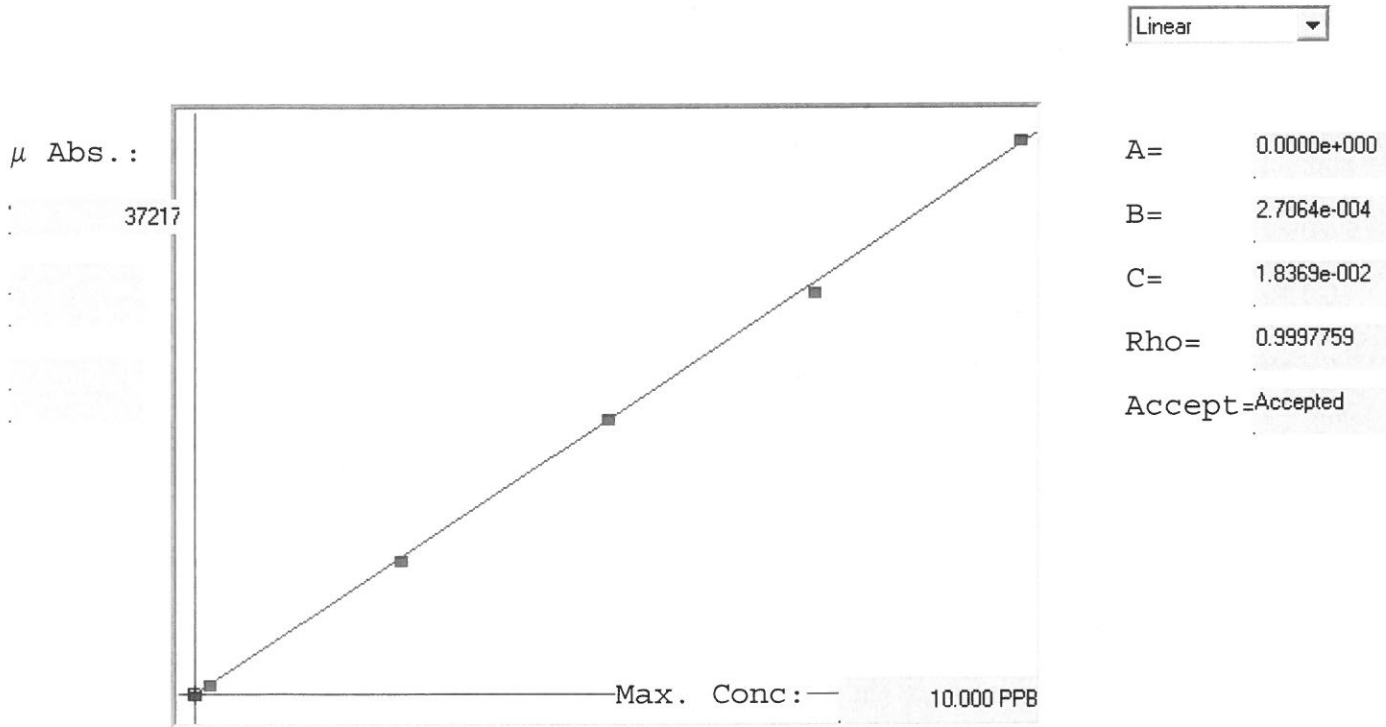

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.024	0.024	19	0.000	19					1
0.2	0.200	0.220	0.020	745	0.0 %	745					10
2.5	2.500	2.460	-0.040	9023	0.0 %	9023					-2
5.0	5.000	5.056	0.056	18613	0.0 %	18613					1
7.5	7.500	7.349	-0.151	27087	0.0 %	27087					-2
10.0	10.000	10.091	0.091	37217	0.0 %	37217					1

LB115192 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Jul 2021 11:33:38

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	19	-	0.00007470A	PPB	02 Jul 2021 11:40:22	S	Std
0.2 - 1	50.2	745	-	0.20007470A	PPB	02 Jul 2021 11:42:39	S	Std
2.5 - 1	52.5	9023	-	2.50007470A	PPB	02 Jul 2021 11:44:55	S	Std
5.0 - 1	55	18613	-	5.00007470A	PPB	02 Jul 2021 11:47:12	S	Std
7.5 - 1	57.5	27087	-	7.50007470A	PPB	02 Jul 2021 11:49:29	S	Std
10.0 - 1	59	37217	-	10.00007470A	PPB	02 Jul 2021 11:51:44	S	Std
ICV87 - 1	ICV87	14026	3.8144	-7470A	PPB	02 Jul 2021 11:54:32	U	SMPL
ICB87 - 1	ICB87	-109	-0.0111	-7470A	PPB	02 Jul 2021 11:56:47	U	SMPL
CCV07 - 1	CCV07	17823	4.8421	-7470A	PPB	02 Jul 2021 11:59:02	U	SMPL
CCB07 - 1	CCB07	-116	-0.0130	-7470A	PPB	02 Jul 2021 12:01:17	U	SMPL
CRA - 1	CRA	650	0.1943	-7470A	PPB	02 Jul 2021 12:03:32	U	SMPL
HighStd - 1	HighStd	35557	9.6417	-7470A	PPB	02 Jul 2021 12:05:47	U	SMPL
ChkStd - 1	ChkStd	24399	6.6218	-7470A	PPB	02 Jul 2021 12:08:02	U	SMPL
PB137475BL - 1	PBW	-181	-0.0306	-7470A	PPB	02 Jul 2021 12:10:19	U	SMPL
PB137475BS - 1	LCSW	14050	3.8209	-7470A	PPB	02 Jul 2021 12:12:35	U	SMPL
M2900-02 - 1	VB16208	-98	-0.0082	-7470A	PPB	02 Jul 2021 12:14:51	U	SMPL
M2901-02 - 1	124035	5	0.0197	-7470A	PPB	02 Jul 2021 12:17:07	U	SMPL
M2901-02DUP - 1	124035DUP	5	0.0197	-7470A	PPB	02 Jul 2021 12:19:24	U	SMPL
M2901-02MS - 1	124035MS	13452	3.6591	-7470A	PPB	02 Jul 2021 12:21:41	U	SMPL
M2901-02MSD - 1	124035MSD	13535	3.6815	-7470A	PPB	02 Jul 2021 12:23:56	U	SMPL
CCV08 - 1	CCV08	18064	4.9073	-7470A	PPB	02 Jul 2021 12:26:11	U	SMPL
CCB08 - 1	CCB08	-116	-0.0130	-7470A	PPB	02 Jul 2021 12:28:26	U	SMPL
M2901-04 - 1	124033	1	0.0186	-7470A	PPB	02 Jul 2021 12:30:42	U	SMPL
M2908-01 - 1	WC-CROPSEY-SOLIDS	-2	0.0178	-7470A	PPB	02 Jul 2021 12:32:58	U	SMPL
PB137476BS - 1	LCSW	13654	3.7137	-7470A	PPB	02 Jul 2021 12:37:28	U	SMPL
M2908-02 - 1	WC-CROPSEY-AQUEOUS	465	0.1442	-7470A	PPB	02 Jul 2021 12:44:33	U	SMPL
M2908-02DUP - 1	WC-CROPSEY-AQUEOUSDUP	455	0.1415	-7470A	PPB	02 Jul 2021 12:46:49	U	SMPL
M2908-02MS - 1	WC-CROPSEY-AQUEOUSMS	13482	3.6672	-7470A	PPB	02 Jul 2021 12:49:05	U	SMPL
M2908-02MSD - 1	WC-CROPSEY-AQUEOUSMSD	13756	3.7413	-7470A	PPB	02 Jul 2021 12:51:22	U	SMPL
PB137476BL - 1	PBW	-85	-0.0046	-7470A	PPB	02 Jul 2021 12:53:39	U	SMPL
CCV09 - 1	CCV09	17674	4.8017	-7470A	PPB	02 Jul 2021 12:55:54	U	SMPL
CCB09 - 1	CCB09	-105	-0.0100	-7470A	PPB	02 Jul 2021 12:58:10	U	SMPL
PB137475TB - 1	PB137448TB	-6	0.0167	-7470A	PPB	02 Jul 2021 13:00:25	U	SMPL
PB137476TB - 1	PB137453TB	17	0.0230	-7470A	PPB	02 Jul 2021 13:02:41	U	SMPL
M2901-02LX5 - 1		19	0.0235	-7470A	PPB	02 Jul 2021 13:04:56	U	SMPL
M2901-02A - 1		13778	3.7473	-7470A	PPB	02 Jul 2021 13:07:12	U	SMPL
M2908-02LX5 - 1		1	0.0186	-7470A	PPB	02 Jul 2021 13:09:27	U	SMPL
M2908-02A - 1		13531	3.6805	-7470A	PPB	02 Jul 2021 13:11:43	U	SMPL
CCV10 - 1	CCV10	17490	4.7519	-7470A	PPB	02 Jul 2021 13:13:59	U	SMPL
CCB10 - 1	CCB10	-94	-0.0071	-7470A	PPB	02 Jul 2021 13:16:15	U	SMPL