


LB115234

7471B

INSTRUMENT ID: CV1

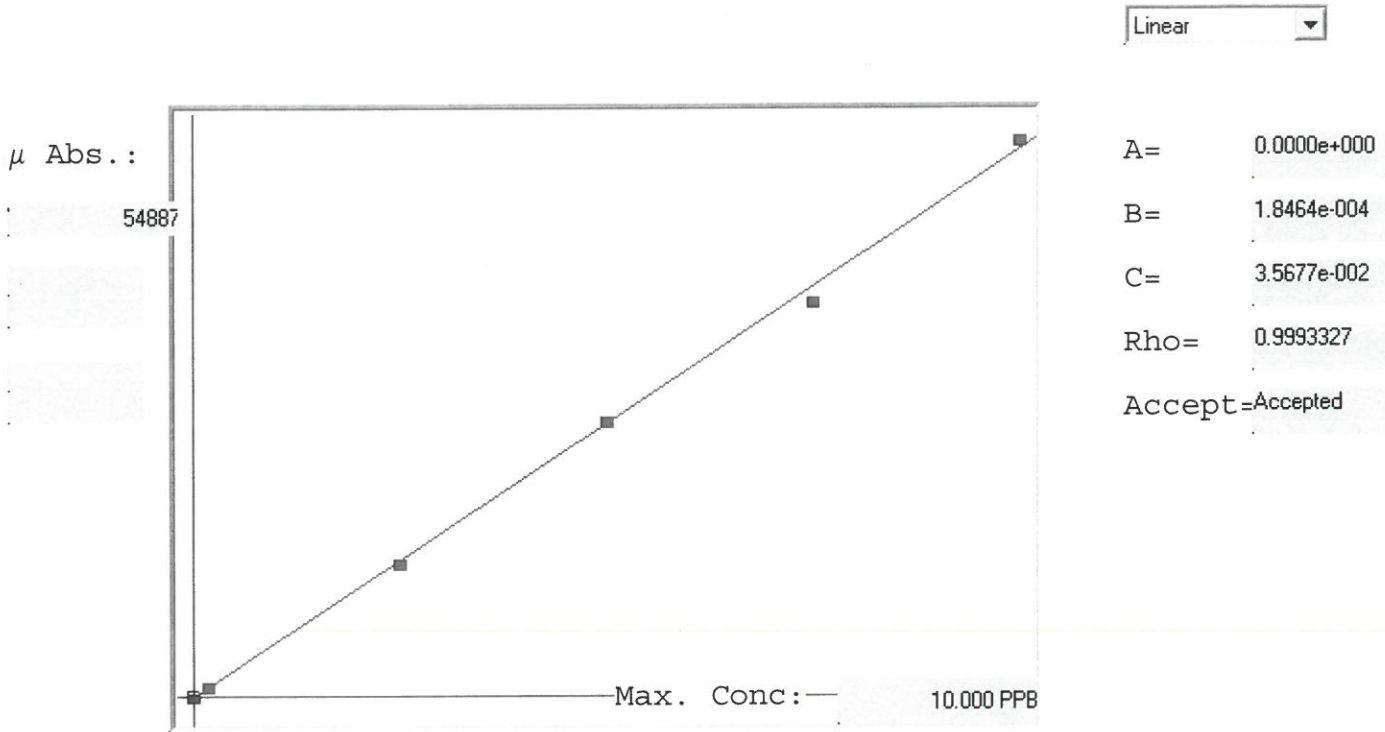

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.043	0.043	38	0.000	38					11
0.2	0.200	0.221	0.021	1004	0.0 %	1004					-1
2.5	2.500	2.485	-0.015	13266	0.0 %	13266					-1
5.0	5.000	5.054	0.054	27178	0.0 %	27178					-4
7.5	7.500	7.227	-0.273	38946	0.0 %	38946					2
10.0	10.000	10.170	0.170	54887	0.0 %	54887					

LB115234 INSTRUMENT ID ; CV1

Method: 7471B

Operator: Admin

Date of Analysis: 07 Jul 2021 15:37:32

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	38	-	0.0000	7471B	PPB	07 Jul 2021 15:38:24	S	Std
0.2 - 1	50.2	1004	-	0.2000	7471B	PPB	07 Jul 2021 15:40:41	S	Std
2.5 - 1	52.5	13266	-	2.5000	7471B	PPB	07 Jul 2021 15:42:58	S	Std
5.0 - 1	55	27178	-	5.0000	7471B	PPB	07 Jul 2021 15:45:14	S	Std
7.5 - 1	57.5	38946	-	7.5000	7471B	PPB	07 Jul 2021 15:47:31	S	Std
10.0 - 1	510	54887	-	10.0000	7471B	PPB	07 Jul 2021 15:52:20	S	Std
ICV93 - 1	ICV93	20198	3.7651	-	7471B	PPB	07 Jul 2021 15:55:10	U	SMPL
ICB93 - 1	ICB93	-105	0.0163	-	7471B	PPB	07 Jul 2021 15:57:24	U	SMPL
CCV27 - 1	CCV27	27346	5.0850	-	7471B	PPB	07 Jul 2021 15:59:40	U	SMPL
CCB27 - 1	CCB27	-111	0.0152	-	7471B	PPB	07 Jul 2021 16:01:55	U	SMPL
CRA - 1	CRA	974	0.2155	-	7471B	PPB	07 Jul 2021 16:04:11	U	SMPL
HighStd - 1	HighStd	54771	10.1489	-	7471B	PPB	07 Jul 2021 16:06:26	U	SMPL
ChkStd - 1	ChkStd	36457	6.7673	-	7471B	PPB	07 Jul 2021 16:08:41	U	SMPL
PB137557BL - 1	PBS	-160	0.0061	-	7471B	PPB	07 Jul 2021 16:10:59	U	SMPL
PB137557BS - 1	LCSS	21472	4.0004	-	7471B	PPB	07 Jul 2021 16:13:16	U	SMPL
M2944-01 - 1	BU-03-070621	1097	0.2382	-	7471B	PPB	07 Jul 2021 16:15:32	U	SMPL
M2946-01 - 1	SB-1	773	0.1784	-	7471B	PPB	07 Jul 2021 16:17:48	U	SMPL
M2946-02 - 1	SB-2	2273	0.4554	-	7471B	PPB	07 Jul 2021 16:20:05	U	SMPL
M2946-03 - 1	SB-3	18525	3.4562	-	7471B	PPB	07 Jul 2021 16:22:22	U	SMPL
M2946-04 - 1	SB-4	69	0.0484	-	7471B	PPB	07 Jul 2021 16:24:37	U	SMPL
CCV28 - 1	CCV28	26959	5.0135	-	7471B	PPB	07 Jul 2021 16:26:52	U	SMPL
CCB28 - 1	CCB28	-109	0.0156	-	7471B	PPB	07 Jul 2021 16:29:08	U	SMPL
M2946-05 - 1	SB-5	438	0.1166	-	7471B	PPB	07 Jul 2021 16:31:23	U	SMPL
M2946-06 - 1	SB-6	160	0.0652	-	7471B	PPB	07 Jul 2021 16:33:38	U	SMPL
M2947-01 - 1	SOIL-BANK-1	157	0.0647	-	7471B	PPB	07 Jul 2021 16:35:53	U	SMPL
M2947-02 - 1	SOIL-BANK-2	472	0.1228	-	7471B	PPB	07 Jul 2021 16:38:09	U	SMPL
M2947-03 - 1	SOIL-BANK-3	377	0.1053	-	7471B	PPB	07 Jul 2021 16:40:25	U	SMPL
M2947-04 - 1	SOIL-BANK-4	249	0.0817	-	7471B	PPB	07 Jul 2021 16:42:41	U	SMPL
M2947-05 - 1	SOIL-BANK-5	514	0.1306	-	7471B	PPB	07 Jul 2021 16:44:58	U	SMPL
M2947-06 - 1	SOIL-BANK-6	1559	0.3235	-	7471B	PPB	07 Jul 2021 16:47:15	U	SMPL
M2947-07 - 1	SOIL-PILE-7	1114	0.2414	-	7471B	PPB	07 Jul 2021 16:49:32	U	SMPL
M2947-08 - 1	SOIL-PILE-8	991	0.2187	-	7471B	PPB	07 Jul 2021 16:51:47	U	SMPL
CCV29 - 1	CCV29	26972	5.0159	-	7471B	PPB	07 Jul 2021 16:54:03	U	SMPL
CCB29 - 1	CCB29	-89	0.0192	-	7471B	PPB	07 Jul 2021 16:56:18	U	SMPL
M2947-09 - 1	SOIL-PILE-9	1080	0.2351	-	7471B	PPB	07 Jul 2021 16:58:34	U	SMPL
M2947-10 - 1	A4-SOIL-BANK	109	0.0558	-	7471B	PPB	07 Jul 2021 17:00:49	U	SMPL
M2947-11 - 1	B6-SOIL-BANK	1789	0.3660	-	7471B	PPB	07 Jul 2021 17:03:05	U	SMPL
M2947-12 - 1	C7-SOIL-PILE	944	0.2100	-	7471B	PPB	07 Jul 2021 17:05:20	U	SMPL
M2947-13 - 1	D9-SOIL-PILE	1215	0.2600	-	7471B	PPB	07 Jul 2021 17:07:36	U	SMPL
M2947-13DUP - 1	D9-SOIL-PILEDUP	1190	0.2554	-	7471B	PPB	07 Jul 2021 17:09:52	U	SMPL
M2947-13MS - 1	D9-SOIL-PILEMS	22397	4.1712	-	7471B	PPB	07 Jul 2021 17:12:09	U	SMPL
M2947-13MSD - 1	D9-SOIL-PILEMSD	21541	4.0131	-	7471B	PPB	07 Jul 2021 17:14:26	U	SMPL
M2947-13LX5 - 1		151	0.0636	-	7471B	PPB	07 Jul 2021 17:16:43	U	SMPL
M2947-13A - 1		21416	3.9900	-	7471B	PPB	07 Jul 2021 17:18:58	U	SMPL
CCV30 - 1	CCV30	26866	4.9963	-	7471B	PPB	07 Jul 2021 17:21:14	U	SMPL
CCB30 - 1	CCB30	-85	0.0200	-	7471B	PPB	07 Jul 2021 17:23:29	U	SMPL