


LB115259

7471B

INSTRUMENT ID: CV1

Linear

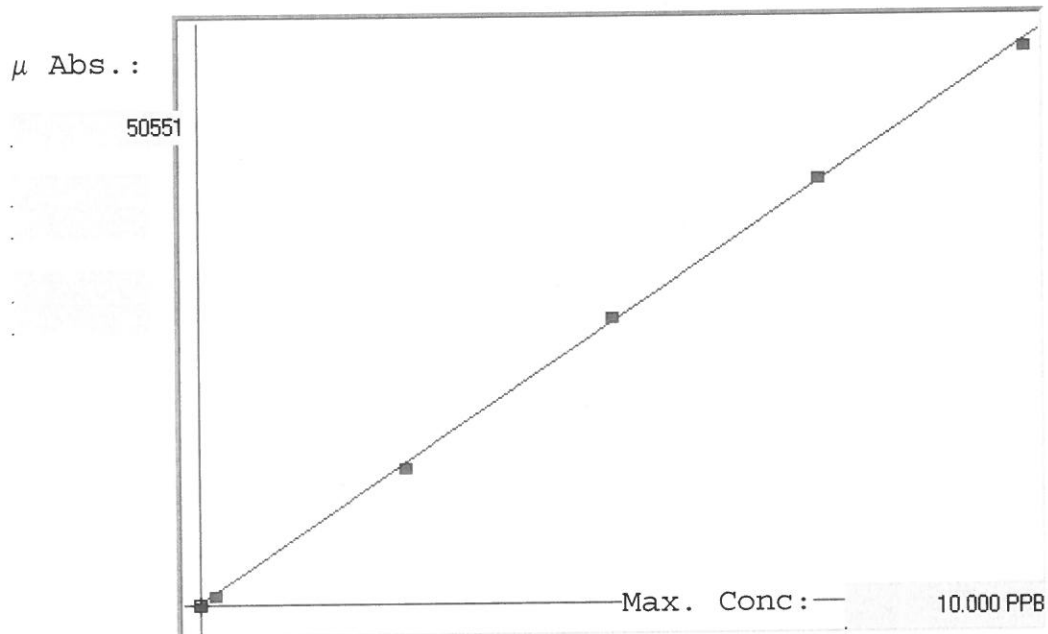

A= 0.0000e+000

B= 1.9621e-004

C= -1.3023e-002

Rho= 0.9998254

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/p)
0.0	0.000	-0.005	-0.005	40	0.000	40					-9
0.2	0.200	0.183	-0.017	998	0.0 %	998					-2
2.5	2.500	2.441	-0.059	12506	0.0 %	12506					2
5.0	5.000	5.101	0.101	26065	0.0 %	26065					1
7.5	7.500	7.575	0.075	38670	0.0 %	38670					-1
10.0	10.000	9.906	-0.094	50551	0.0 %	50551					

LB115259 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 08 Jul 2021 13:53:30					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	40	-	0.0000	7471B	PPB	08 Jul 2021 13:59:17	S	Std
0.2 - 1	50.2	998	-	0.2000	7471B	PPB	08 Jul 2021 14:01:33	S	Std
2.5 - 1	52.5	12506	-	2.5000	7471B	PPB	08 Jul 2021 14:03:50	S	Std
5.0 - 1	55	26065	-	5.0000	7471B	PPB	08 Jul 2021 14:06:07	S	Std
7.5 - 1	57.5	38670	-	7.5000	7471B	PPB	08 Jul 2021 14:08:23	S	Std
10.0 - 1	510	50551	-	10.0000	7471B	PPB	08 Jul 2021 14:10:40	S	Std
ICV94 - 1	ICV94	20295	3.9691	-	7471B	PPB	08 Jul 2021 14:13:32	U	SMPL
ICB94 - 1	ICB94	-77	-0.0281	-	7471B	PPB	08 Jul 2021 14:15:46	U	SMPL
CCV31 - 1	CCV31	25591	5.0083	-	7471B	PPB	08 Jul 2021 14:18:01	U	SMPL
CCB31 - 1	CCB31	-91	-0.0309	-	7471B	PPB	08 Jul 2021 14:20:15	U	SMPL
CRA - 1	CRA	977	0.1787	-	7471B	PPB	08 Jul 2021 14:22:31	U	SMPL
HighStd - 1	HighStd	49908	9.7796	-	7471B	PPB	08 Jul 2021 14:24:46	U	SMPL
ChkStd - 1	ChkStd	35794	7.0102	-	7471B	PPB	08 Jul 2021 14:27:01	U	SMPL
PB137580BL - 1	PBS	-154	-0.0432	-	7471B	PPB	08 Jul 2021 14:29:19	U	SMPL
PB137580BS - 1	LCSS	17487	3.4182	-	7471B	PPB	08 Jul 2021 14:31:35	U	SMPL
M2956-01 - 1	RO-72-12000-ETGI-283	1326	0.2472	-	7471B	PPB	08 Jul 2021 14:38:45	U	SMPL
M2956-01DUP - 1	RO-72-12000-ETGI-283DUP	1241	0.2305	-	7471B	PPB	08 Jul 2021 14:41:01	U	SMPL
M2956-01MS - 1	RO-72-12000-ETGI-283MS	18792	3.6742	-	7471B	PPB	08 Jul 2021 14:43:18	U	SMPL
M2956-01MSD - 1	RO-72-12000-ETGI-283MSD	19151	3.7447	-	7471B	PPB	08 Jul 2021 14:45:35	U	SMPL
M2963-01 - 1	MH-2A-COMP	475	0.0802	-	7471B	PPB	08 Jul 2021 14:47:49	U	SMPL
CCV32 - 1	CCV32	25167	4.9251	-	7471B	PPB	08 Jul 2021 14:50:04	U	SMPL
CCB32 - 1	CCB32	-77	-0.0281	-	7471B	PPB	08 Jul 2021 14:52:19	U	SMPL
M2963-03 - 1	MH-2B-COMP	791	0.1422	-	7471B	PPB	08 Jul 2021 14:54:35	U	SMPL
M2963-05 - 1	MH-1A-COMP	2156	0.4100	-	7471B	PPB	08 Jul 2021 14:56:51	U	SMPL
M2963-07 - 1	MH-1B-COMP	2139	0.4067	-	7471B	PPB	08 Jul 2021 14:59:06	U	SMPL
M2965-01 - 1	RO-ETGI-345	11240	2.1924	-	7471B	PPB	08 Jul 2021 15:01:21	U	SMPL
M2967-01 - 1	1-5ft-GRACE-AVE-TP-1	621	0.1088	-	7471B	PPB	08 Jul 2021 15:03:37	U	SMPL
M2967-05 - 1	1-8FT-STEFANIC-AVE-TP-2	1485	0.2784	-	7471B	PPB	08 Jul 2021 15:05:53	U	SMPL
M2967-09 - 1	1-5FT-CADMUS-AVE-TP-3	730	0.1302	-	7471B	PPB	08 Jul 2021 15:08:10	U	SMPL
M2956-01LX5 - 1		263	0.0386	-	7471B	PPB	08 Jul 2021 15:10:27	U	SMPL
M2956-01A - 1		20368	3.9834	-	7471B	PPB	08 Jul 2021 15:12:44	U	SMPL
CCV33 - 1	CCV33	25214	4.9343	-	7471B	PPB	08 Jul 2021 15:14:59	U	SMPL
CCB33 - 1	CCB33	-77	-0.0281	-	7471B	PPB	08 Jul 2021 15:17:14	U	SMPL