


LB115309

7471B

INSTRUMENT ID: CV1

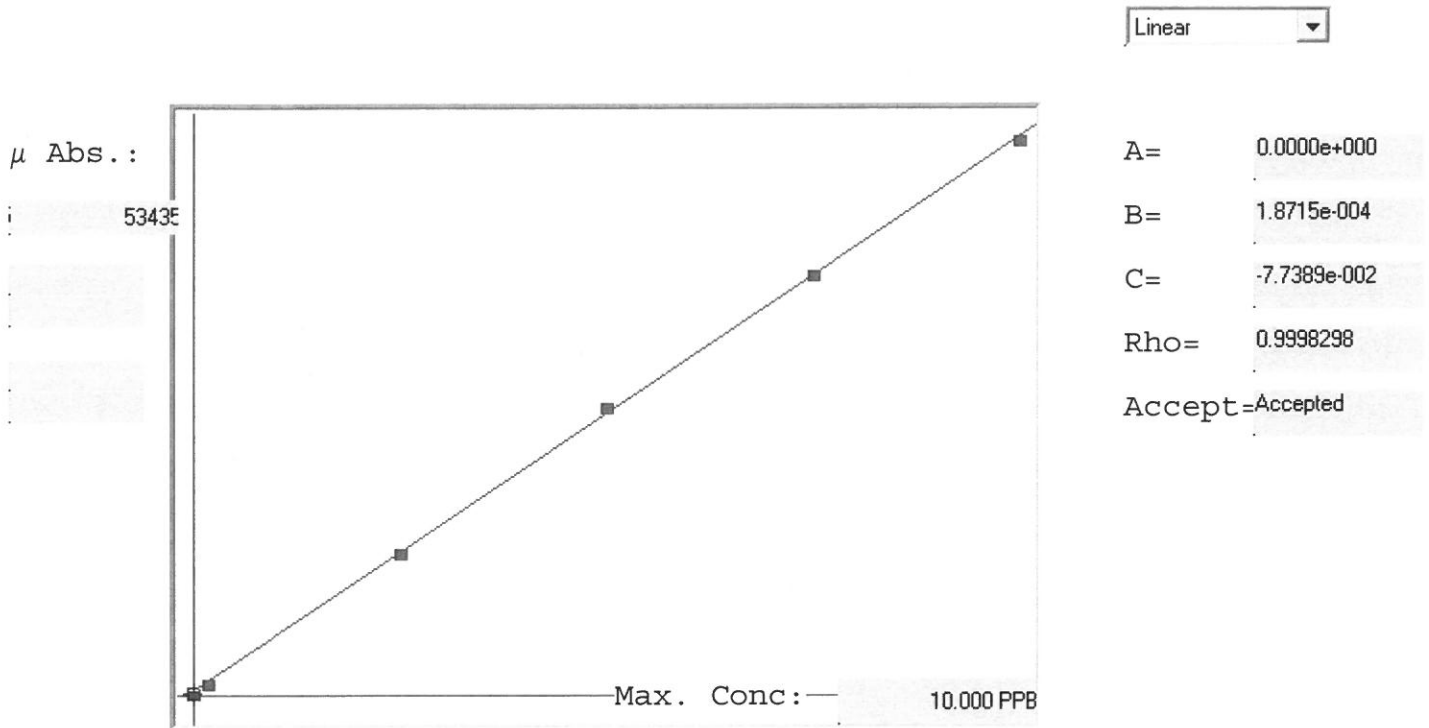

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	abd
0.0	0.000	-0.023	-0.023	292	0.000	292					-20
0.2	0.200	0.161	-0.039	1276	0.0 %	1276					0
2.5	2.500	2.488	-0.012	13705	0.0 %	13705					3
5.0	5.000	5.140	0.140	27878	0.0 %	27878					0
7.5	7.500	7.511	0.011	40546	0.0 %	40546					0
10.0	10.000	9.923	-0.077	53435	0.0 %	53435					-1

LB115309 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 12 Jul 2021 16:08:49

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	292	-	0.0000	7471B	PPB	12 Jul 2021 16:10:07	S	Std
0.2 - 1	50.2	1276	-	0.2000	7471B	PPB	12 Jul 2021 16:12:24	S	Std
2.5 - 1	52.5	13705	-	2.5000	7471B	PPB	12 Jul 2021 16:14:41	S	Std
5.0 - 1	55	27878	-	5.0000	7471B	PPB	12 Jul 2021 16:16:57	S	Std
7.5 - 1	57.5	40546	-	7.5000	7471B	PPB	12 Jul 2021 16:19:14	S	Std
10.0 - 1	59.0	53435	-	10.0000	7471B	PPB	12 Jul 2021 16:21:32	S	Std
ICV01 - 1	ICV01	21342	3.9168	-7471B	PPB	PPB	12 Jul 2021 16:24:10	U	SMPL
ICB01 - 1	ICB01	96	-0.0594	-7471B	PPB	PPB	12 Jul 2021 16:26:25	U	SMPL
CCV50 - 1	CCV50	28183	5.1971	-7471B	PPB	PPB	12 Jul 2021 16:28:40	U	SMPL
CCB50 - 1	CCB50	87	-0.0611	-7471B	PPB	PPB	12 Jul 2021 16:30:55	U	SMPL
CRA - 1	CRA	1256	0.1577	-7471B	PPB	PPB	12 Jul 2021 16:33:11	U	SMPL
HighStd - 1	HighStd	53579	9.9500	-7471B	PPB	PPB	12 Jul 2021 16:35:26	U	SMPL
ChkStd - 1	ChkStd	38020	7.0381	-7471B	PPB	PPB	12 Jul 2021 16:37:41	U	SMPL
PB137626BL - 1	PBS	145	-0.0503	-7471B	PPB	PPB	12 Jul 2021 16:42:31	U	SMPL
PB137626BS - 1	LCSS	18410	3.3681	-7471B	PPB	PPB	12 Jul 2021 16:44:47	U	SMPL
M2997-01 - 1	RBR-200029	90066	16.7785	-7471B	PPB	PPB	12 Jul 2021 16:47:03	U	SMPL
M2998-01 - 1	VNJ-231	11664	2.1055	-7471B	PPB	PPB	12 Jul 2021 16:49:19	U	SMPL
M3001-01 - 1	CHRT-25720	6671	1.1711	-7471B	PPB	PPB	12 Jul 2021 16:51:38	U	SMPL
M3001-03 - 1	N9994	2279	0.3491	-7471B	PPB	PPB	12 Jul 2021 16:53:55	U	SMPL
M3001-03DUP - 1	N9994DUP	2442	0.3796	-7471B	PPB	PPB	12 Jul 2021 16:56:11	U	SMPL
CCV51 - 1	CCV51	28142	5.1894	-7471B	PPB	PPB	12 Jul 2021 16:58:26	U	SMPL
CCB51 - 1	CCB51	92	-0.0602	-7471B	PPB	PPB	12 Jul 2021 17:00:41	U	SMPL
M3001-03MS - 1	N9994MS	22505	4.1344	-7471B	PPB	PPB	12 Jul 2021 17:02:57	U	SMPL
M3001-03MSD - 1	N9994MSD	23376	4.2974	-7471B	PPB	PPB	12 Jul 2021 17:07:42	U	SMPL
M3002-01 - 1	TP-F	1563	0.2151	-7471B	PPB	PPB	12 Jul 2021 17:09:56	U	SMPL
M3002-04 - 1	TP-H	837	0.0793	-7471B	PPB	PPB	12 Jul 2021 17:12:12	U	SMPL
M3006-01 - 1	CL-02-070921	1956	0.2887	-7471B	PPB	PPB	12 Jul 2021 17:14:28	U	SMPL
M3001-03LX5 - 1		618	0.0383	-7471B	PPB	PPB	12 Jul 2021 17:16:45	U	SMPL
M3001-03A - 1		24126	4.4378	-7471B	PPB	PPB	12 Jul 2021 17:19:01	U	SMPL
M2997-01DLX5 - 1		18838	3.4482	-7471B	PPB	PPB	12 Jul 2021 17:21:18	U	SMPL
CCV52 - 1	CCV52	28068	5.1756	-7471B	PPB	PPB	12 Jul 2021 17:23:59	U	SMPL
CCB52 - 1	CCB52	95	-0.0596	-7471B	PPB	PPB	12 Jul 2021 17:26:15	U	SMPL