

LB115349


7470A

INSTRUMENT ID: CVJ

Linear

 μ Abs.:

38375

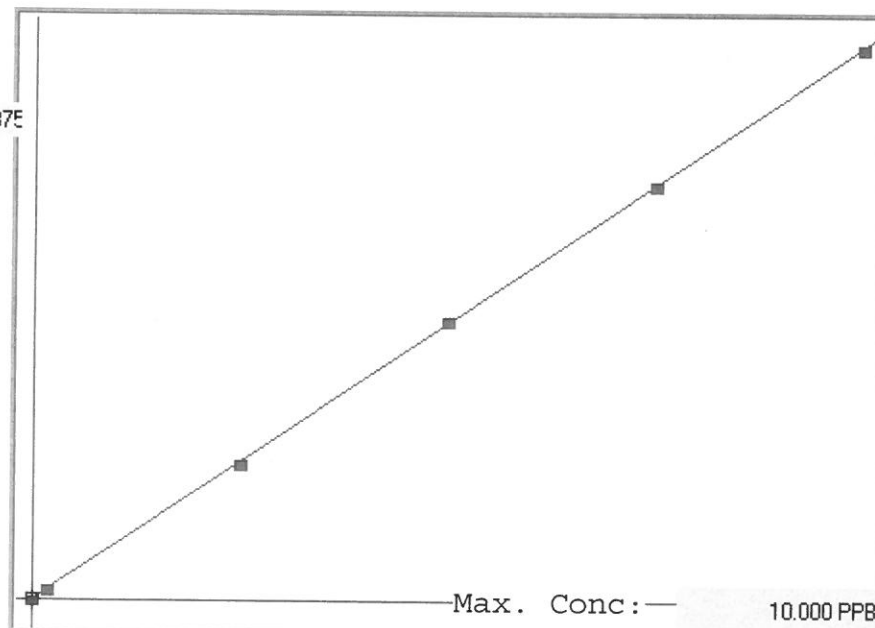

A= 0.0000e+000

B= 2.5991e-004

C= -2.4263e-003

Rho= 0.9999504

Accept=Accepted

td ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	('/b)
.0	0.000	0.012	0.012	57	0.000	57					-
.2	0.200	0.188	-0.012	733	0.0 %	733					-6
.5	2.500	2.452	-0.048	9444	0.0 %	9444					-2
.0	5.000	5.068	0.068	19509	0.0 %	19509					1
.5	7.500	7.508	0.008	28896	0.0 %	28896					0
0.0	10.000	9.971	-0.029	38375	0.0 %	38375					0

LB115349 INSTRUMENT ID :CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Jul 2021 13:08:56

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	57	-	0.0000	7470A	PPB	14 Jul 2021 13:56:45	S	Std
0.2 - 1	SO-2	733	-	0.2000	7470A	PPB	14 Jul 2021 13:59:02	S	Std
2.5 - 1	SO-5	9444	-	2.5000	7470A	PPB	14 Jul 2021 14:01:19	S	Std
5.0 - 1	SO	19509	-	5.0000	7470A	PPB	14 Jul 2021 14:03:36	S	Std
7.5 - 1	SO-5	28896	-	7.5000	7470A	PPB	14 Jul 2021 14:09:08	S	Std
10.0 - 1	SO	38375	-	10.0000	7470A	PPB	14 Jul 2021 14:13:54	S	Std
ICV04 - 1	ICV04	15315	3.9780	-7470A	PPB	14 Jul 2021 14:16:33	U	SMPL	
ICB04 - 1	ICB04	-50	-0.0154	-7470A	PPB	14 Jul 2021 14:18:47	U	SMPL	
CCV60 - 1	CCV60	19856	5.1583	-7470A	PPB	14 Jul 2021 14:21:02	U	SMPL	
CCB60 - 1	CCB60	-64	-0.0191	-7470A	PPB	14 Jul 2021 14:23:17	U	SMPL	
CRA - 1	CRA	730	0.1873	-7470A	PPB	14 Jul 2021 14:25:32	U	SMPL	
HighStd - 1	HighStd	38020	9.8792	-7470A	PPB	14 Jul 2021 14:27:47	U	SMPL	
ChkStd - 1	ChkStd	26731	6.9451	-7470A	PPB	14 Jul 2021 14:30:02	U	SMPL	
PB137691BL - 1	PBW	-145	-0.0401	-7470A	PPB	14 Jul 2021 14:32:19	U	SMPL	
PB137691BS - 1	LCSW	16105	4.1834	-7470A	PPB	14 Jul 2021 14:34:35	U	SMPL	
M3021-01 - 1	31455	-80	-0.0232	-7470A	PPB	14 Jul 2021 14:36:51	U	SMPL	
M3021-03 - 1	31456	20	0.0028	-7470A	PPB	14 Jul 2021 14:39:07	U	SMPL	
M3025-01 - 1	070921HU01	569	0.1455	-7470A	PPB	14 Jul 2021 14:41:24	U	SMPL	
M3026-03 - 1	ABN-JG-1	-20	-0.0076	-7470A	PPB	14 Jul 2021 14:43:41	U	SMPL	
M3026-06 - 1	ABN-JG-2	37	0.0072	-7470A	PPB	14 Jul 2021 14:45:56	U	SMPL	
CCV61 - 1	CCV61	19593	5.0899	-7470A	PPB	14 Jul 2021 14:48:11	U	SMPL	
CCB61 - 1	CCB61	-29	-0.0100	-7470A	PPB	14 Jul 2021 14:50:26	U	SMPL	
M3026-09 - 1	ABN-JG-3	33	0.0062	-7470A	PPB	14 Jul 2021 14:52:41	U	SMPL	
M3026-12 - 1	ABN-JG-4	49	0.0103	-7470A	PPB	14 Jul 2021 14:54:56	U	SMPL	
M3027-01 - 1	NWB-1572	50	0.0106	-7470A	PPB	14 Jul 2021 14:57:12	U	SMPL	
M3027-01DUP - 1	NWB-1572DUP	63	0.0139	-7470A	PPB	14 Jul 2021 14:59:28	U	SMPL	
M3027-01MS - 1	NWB-1572MS	16391	4.2577	-7470A	PPB	14 Jul 2021 15:01:44	U	SMPL	
M3027-01MSD - 1	NWB-1572MSD	14325	3.7207	-7470A	PPB	14 Jul 2021 15:04:00	U	SMPL	
PB137692BL - 1	PBW	-51	-0.0157	-7470A	PPB	14 Jul 2021 15:06:17	U	SMPL	
PB137692BS - 1	LCSW	15024	3.9024	-7470A	PPB	14 Jul 2021 15:08:34	U	SMPL	
M3027-03 - 1	NWB-1639	168	0.0412	-7470A	PPB	14 Jul 2021 15:10:51	U	SMPL	
M3027-03DUP - 1	NWB-1639DUP	51	0.0108	-7470A	PPB	14 Jul 2021 15:15:45	U	SMPL	
CV62 - 1	CCV62	20041	5.2064	-7470A	PPB	14 Jul 2021 15:18:00	U	SMPL	
CB62 - 1	CCB62	-54	-0.0165	-7470A	PPB	14 Jul 2021 15:20:15	U	SMPL	
M3027-03MS - 1	NWB-1639MS	15409	4.0025	-7470A	PPB	14 Jul 2021 15:25:55	U	SMPL	
M3027-03MSD - 1	NWB-1639MSD	15448	4.0126	-7470A	PPB	14 Jul 2021 15:28:10	U	SMPL	
M3027-05 - 1	NWB-1640	-28	-0.0097	-7470A	PPB	14 Jul 2021 15:30:25	U	SMPL	
B137691TB - 1	PB137667TB	-5	-0.0037	-7470A	PPB	14 Jul 2021 15:32:42	U	SMPL	
B137692TB - 1	PB137670TB	23	0.0036	-7470A	PPB	14 Jul 2021 15:34:57	U	SMPL	
M3027-01LX5 - 1		59	0.0129	-7470A	PPB	14 Jul 2021 15:40:33	U	SMPL	
M3027-01A - 1		15643	4.0633	-7470A	PPB	14 Jul 2021 15:42:49	U	SMPL	
M3027-03LX5 - 1		1	-0.0022	-7470A	PPB	14 Jul 2021 15:45:06	U	SMPL	
M3027-03A - 1		15258	3.9632	-7470A	PPB	14 Jul 2021 15:47:23	U	SMPL	
CV63 - 1	CCV63	19444	5.0512	-7470A	PPB	14 Jul 2021 15:49:38	U	SMPL	
CB63 - 1	CCB63	-67	-0.0198	-7470A	PPB	14 Jul 2021 15:51:54	U	SMPL	